



Laboratory Services Materials (Trace Evidence)

These are management system documents utilized by ATF Laboratories. They are provided for informational purposes only. Sensitive or copyrighted information has been redacted. The documents are used in ATF Laboratories and not published with the intent of setting a policy or analysis standard for other laboratories. The inclusion of product names does not imply endorsement by ATF Laboratories.

These documents are current as of April 20, 2023. ATF management system documents are reviewed annually and revised as needed. For specific requests, submit a Freedom of Information Act (FOIA) request. Instructions on how to file a FOIA request are found at: www.atf.gov/resource-center/freedom-information-act-foia.

INDEX

- ATF-LS-TE00 Standard Approach for Examinations of Trace Evidence
- ATF-LS-TE01 Setup and Use of Fluorescence Microscopy
- ATF-LS-TE02 Setup and Use of the Microscope
- ATF-LS-TE03 Use of the Microspectrophotometer
- ATF-LS-TE04 Pyrolysis-Gas Chromatography Mass Spectrometry
- ATF-LS-TE07 Raman Spectrometer
- ATF-LS-TE09 Examination and Analysis of Hair Evidence
- ATF-LS-TE10 Examination of Physical Fits
- ATF-LS-TE11 Examination, Analysis, and Comparison of Textile Fibers
- ATF-LS-TE13 Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives
- ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence
- ATF-LS-TE15 Examination, Analysis, and Comparison of Paint
- ATF-LS-TE16 Report Writing
- ATF-LS-TE17 Trace Abbreviations



ATF-LS-TE00 - Standard Approach to the Examination of Trace Evidence	ID: 11780 Revision: 1
Authority: Deputy Assistant Director, Forensic Services	Page: 1 of 2
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

- 1.1. This document describes the general approach to trace evidence examinations.
- 1.2. The Trace Section performs analyses on a wide variety of materials, some of which include fibers, hairs, paints, polymers, and tape.
- 1.3. This document is not meant to encompass all possible circumstances that may be encountered in forensic casework, nor is it a step-by-step process, as different types of trace evidence require different procedures. The selection of material(s) for analysis and the analytical scheme is determined by the examiner and is case-dependent.


2. Processing Physical Evidence

- 2.1. A general examination approach includes a visual examination of the item of evidence followed by a microscopic examination.
- 2.2. The evidence must be clearly documented in the technical record which can include photographs, sketches and/or written descriptions. See *ATF-LS-7.5 Technical records*
- 2.3. Each item should be examined separately (by time and/or space) unless items are packaged together. Ensure good laboratory practices are followed to minimize the potential of cross-transfer and/or contamination.
- 2.4. Different types of illumination (e.g., oblique lighting, lit magnifier, alternate light sources) can be used to detect trace evidence.
- 2.5. Collection techniques such as particle picking, scraping, brushing, tape lifting, etc., can be used if the visual and microscopical examinations warrant it.
- 2.6. Any materials of interest (for further examination and/or comparison) are separated and protected from alteration, contamination, or loss.
- 2.7. When a comparative examination is requested, the questioned item is evaluated to identify characteristics suitable for comparison prior to examination of the known item. In certain circumstances, it may be appropriate to perform a preliminary characterization of the known prior to the assessment of the unknown (e.g., determining fiber color of known prior to searching for fibers on a tape-lift).

3. General Evidence Examination (see flowchart)



General Trace Evidence Flow Chart

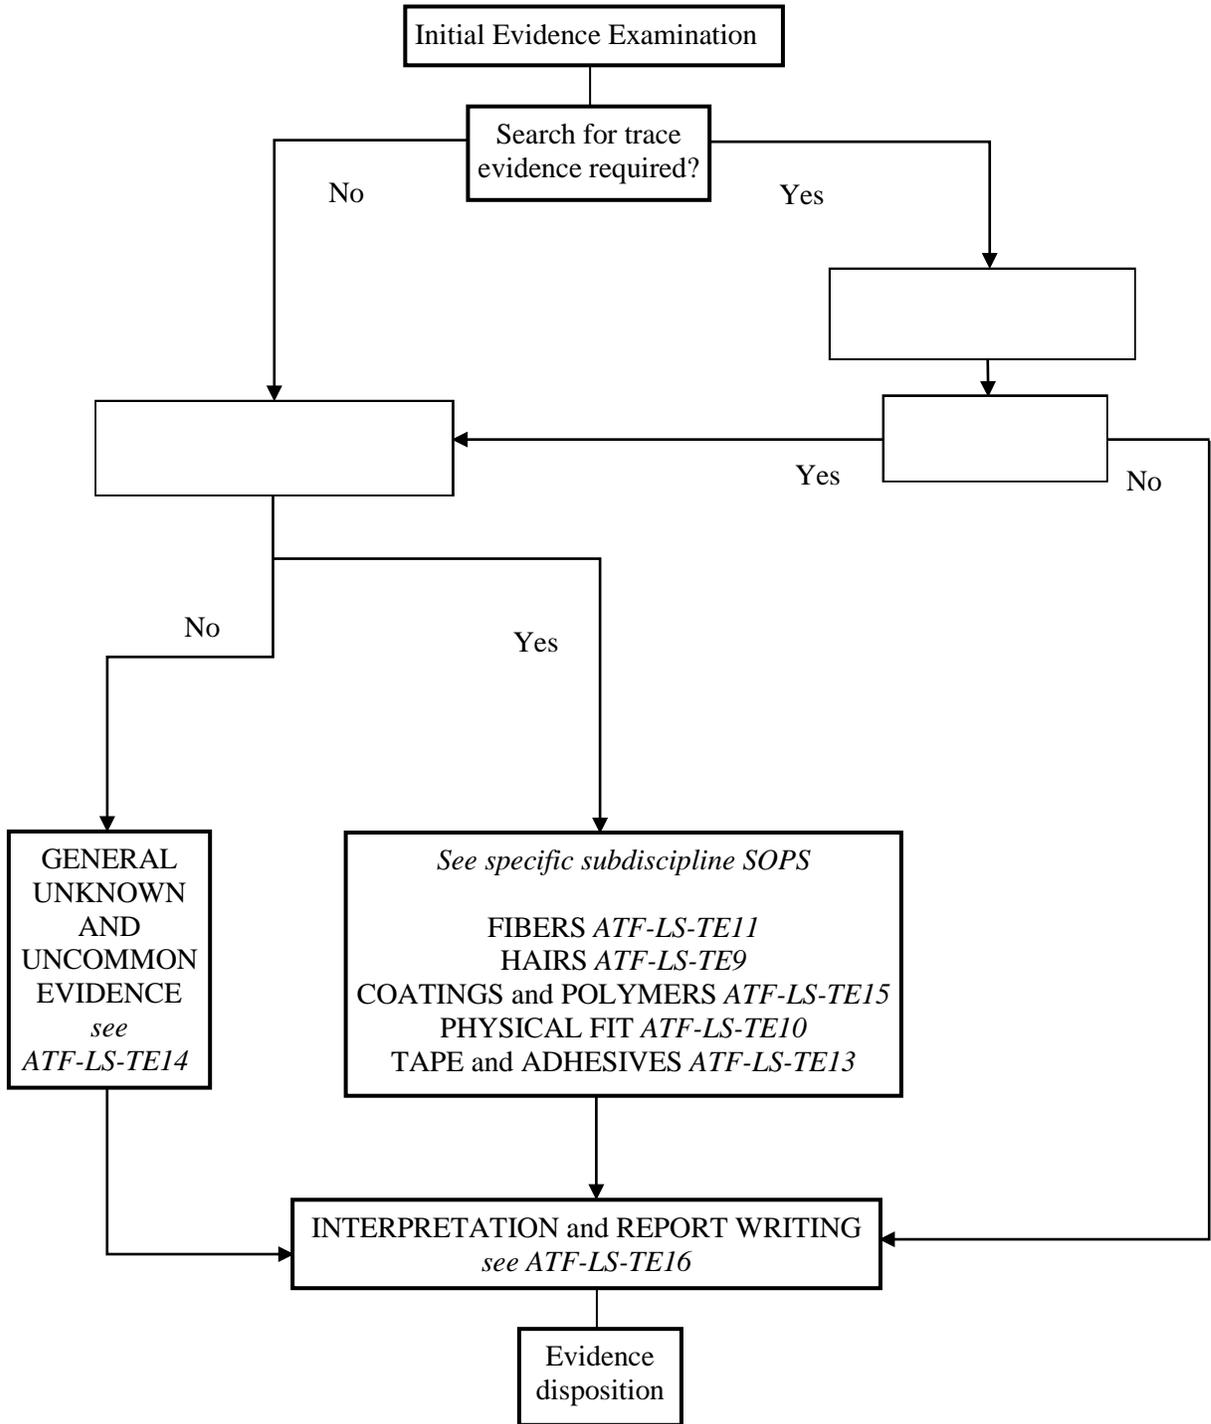



ATF-LS-TE01 – Setup and Use of Fluorescence Microscopy	ID: 1920 Revision: 5
Authority: Technical Leader	Page: 1 of 4
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

1.1. This method describes the procedure for setup and use of the reflected light fluorescence attachment on the polarized light microscope (PLM). Fluorescence microscopy is utilized for detecting and characterizing fluorescing substances in materials such as pigments in paints and for comparing fibers that have fluorescing dyes or optical brighteners. The procedure below is for the mercury, xenon, and LED light sources.

2. Instrumentation/Reagents

2.1. Reflected Light Fluorescence Attachment

2.2. Fluorescence Cubes

2.3. Mounting media

3. Safety Considerations

3.1. Follow standard laboratory safety procedures and those recommended in manufacturer's instruction manuals.

3.2. Gloves and safety glasses should be worn when handling the light source.

3.3. Never look directly at the Ultraviolet (UV) light source.

3.4. Allow the lamp housing and lamp to cool before changing a burned-out lamp.

4. Procedure for Analysis

4.1. UV light source alignment and adjustment

4.1.1. The alignment and adjustment shall be conducted whenever the light source is changed or whenever necessary before an examination (e.g., image is partially obscured or unevenly illuminated).

4.1.2. Refer to manufacturer's instructions manual for specific instructions on the adjustment and alignment of the light source.

4.1.3. **Warning:** If using the mercury burner (lamp) the following precautions shall be followed.



ATF-LS-TE01 – Setup and Use of Fluorescence Microscopy	ID: 1920 Revision: 5
Authority: Technical Leader	Page: 2 of 4
Original maintained by Quality Programs; copies are uncontrolled.	

- 4.1.3.1. If the burner does not ignite, turn the main switch off once, and then repeat after 5 or 10 seconds.
- 4.1.3.2. To avoid shortening the life of the burner, do not turn the burner off within 15 minutes of ignition.
- 4.1.3.3. After turning the burner off, it cannot be re-ignited until the mercury vapor cools and condenses to liquid. Wait for about 10 minutes before restarting the burner.

4.1.4. **Warning:** If using the X-cite LED, ensure that the source is kept on until the fan shuts off.

4.2. Reflected Light Fluorescence Observations

- 4.2.1. Close the vertical light path shutter and turn on the UV light source (See 4.1.3 if using the mercury burner).
- 4.2.2. Using the transmitted light source, focus on the specimen using the desired objective.
- 4.2.3. Bring a suitable cube into the light path and turn off the transmitted light source.
- 4.2.4. Open the vertical light shutter and refocus on the specimen, if necessary.
- 4.2.5. Adjust the brightness.
 - 4.2.5.1. Mercury burner: Adjust the collector lens-focusing knob to where the brightness and evenness of the illumination in the field of view are at a maximum. Adjust the aperture diaphragm as needed.
 - 4.2.5.2. LED: Adjust the brightness/intensity and aperture diaphragm as needed.
- 4.2.6. The intensity (e.g., none, low, moderate, high) and the color of the fluorescence shall be noted in the case record.

5. Quality Assurance and Controls

- 5.1. Proper alignment of the microscope is completed when the microscope is initially set up and is readjusted as needed during the examination.



ATF-LS-TE01 – Setup and Use of Fluorescence Microscopy	ID: 1920 Revision: 5
Authority: Technical Leader	Page: 3 of 4
Original maintained by Quality Programs; copies are uncontrolled.	

- 5.2. A sample of known fluorescence shall be examined daily, prior to examining the case-related sample(s). The reference fiber F10.143 from the Microtrace Collection is used and checked under each filter. Only the filters that have a successful performance check will be utilized in casework. The details of the filters as well as the expected color are below for each fluorescent microscope in the laboratory. The results of the performance check shall be documented in the case record.

MICROSCOPE: Leica DM2700		
Filter	Excitation region	Fluorescence
Ultraviolet	340 – 380 nm	Blue
Blue	432.5 – 439.5 nm	Green/blue
Green	515 – 560 nm	Red
Green Fluorescent Protein (GFP)	450 – 490 nm	Green

MICROSCOPE: LEEDS COMPARISON		
Filter	Excitation region	Fluorescence
Ultraviolet	361 - 389 nm	Blue
Blue Violet Narrow	400 – 440 nm	Green/blue
Green Wide	527.5 – 552.5 nm	Red
Blue Narrow	465 – 495 nm	Yellow

MICROSCOPE: Olympus BX60		
Filter	Excitation region	Fluorescence
Ultraviolet	330 – 385 nm	Blue
Blue Violet Narrow	420 – 440 nm	Green
Green Wide	510 – 550 nm	Red
Blue Wide	450 – 480 nm	Yellow

- 5.3. Microscopes should be cleaned and adjusted regularly by a manufacturer's service representative per the service contract agreement. The maintenance shall be documented (e.g., Logbook).
- 5.4. Fluorescence microscopy is a well-known and scientifically accepted method for the analysis and comparison of fluorescing materials in many types of trace evidence. Relevant examples of the broad nature of the method and related literature can be found in Section 6 (References).



ATF-LS-TE01 – Setup and Use of Fluorescence Microscopy	ID: 1920 Revision: 5
Authority: Technical Leader	Page: 4 of 4
Original maintained by Quality Programs; copies are uncontrolled.	

6. References

ASTM E2228 Standard Guide for Microscopical Examination of Textile Fibers

Forensic Examination of Fibres, 3rd Edition. Edited by James Robertson, Claude Roux and Kenneth G. Wiggins. Pages 149, 172-175.

Leica DML Instruction Manual – Incident Light Chapter

Leica DM2700 M: Instructions for use

Leica DM2700 P: Supplement to the instructions for use for Leica DM2700 M

Leeds Forensic Systems, Inc. Optional Reflected Fluorescence Lighting Manual

Olympus BX-FLA Reflected Light Fluorescence Attachment Instruction Manual



ATF-LS-TE02 Setup and Use of the Microscope	ID: 1922 Revision: 6
Authority: Technical Leader	Page: 1 of 7
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

- 1.1. This method describes the procedure for basic microscopy setup on compound polarized light microscopes (PLM), but certain sections can also be used for brightfield (biological) microscopes. Also, the “Ocular Focus Adjustment” and the “Calculation of Ocular Scale Magnification Factors” sections could be used for stereomicroscopes and the “Ocular Focus Adjustment” can be used for the FTIR microscope.
- 1.2. The proper setup of the microscope is important since the PLM is one of the most powerful analytical tools available to the forensic trace examiner. PLM allows an examiner to quickly characterize, identify, and compare particles/fibers encountered in case work by determining a variety of physical and optical properties which include size, morphology, surface texture, color, pleochroism, refractive index (indices), birefringence, sign of elongation, extinction, interference figure, optic sign, and crystal system.

2. Instrumentation/reagents

- 2.1. Brightfield microscope
- 2.2. Comparison microscope
- 2.3. Polarizing light microscope (PLM)
- 2.4. Stereomicroscope
- 2.5. Phase contrast microscope
- 2.6. Micrometer scale

3. Safety considerations

- 3.1. Follow standard laboratory safety procedures.

4. Procedure or analysis

4.1. Sample preparation

- 4.1.1. Pre-cleaned slides can be used, or slides and cover slips can be cleaned with common solvents, such as methanol, ethanol, or glass cleaner; a dry Kimwipe can also be used.



ATF-LS-TE02 Setup and Use of the Microscope	ID: 1922 Revision: 6
Authority: Technical Leader	Page: 2 of 7
Original maintained by Quality Programs; copies are uncontrolled.	

- 4.1.2. Different mounting media can be used to allow the optical properties of a sample to be fully characterized.
 - 4.1.2.1. Some mounting media are semi-permanent, such as Permount, or permanent, like Norland Optical. Note: Norland Optical needs UV light to set. Other mounting mediums are temporary, such as Cargille oils or glycerin mixture (with methanol or water).
 - 4.1.2.2. The lot number and expiration date (if applicable) shall be documented in the examination record if it could affect analysis (e.g., determining refractive index of a fiber).
- 4.1.3. Refer to individual trace evidence sub-discipline procedures for further requirements regarding sample preparation.
- 4.2. Modified Köhler illumination/field diaphragm adjustment
 - 4.2.1. Place a prepared slide on the microscope stage and turn on the microscope.
 - 4.2.2. Adjust the light intensity to a comfortable viewing level and focus on a particle with the 10X objective or an objective of higher magnification.
 - 4.2.3. Make sure the top condenser lens is in position and open the aperture diaphragm on the condenser.
 - 4.2.4. Close down the field diaphragm.
 - 4.2.5. Adjust the condenser height until the image of the field diaphragm (the edges of the diaphragm) is in sharp focus.
 - 4.2.6. Reduce color fringes to a minimum with the aperture diaphragm.
 - 4.2.7. Center the image of the field diaphragm by using the centering screws on the condenser.
 - 4.2.8. Gradually widen the field diaphragm until it leaves the field of view. Adjust the aperture diaphragm as desired for the best resolution/contrast.
 - 4.2.9. Readjust the light intensity to a comfortable viewing level.
- 4.3. Lamp adjustment



ATF-LS-TE02 Setup and Use of the Microscope	ID: 1922 Revision: 6
Authority: Technical Leader	Page: 3 of 7
Original maintained by Quality Programs; copies are uncontrolled.	

4.3.1. Refer to the manufacturer's manual for the procedure regarding the focusing and centering of the microscope lamp.

4.4. Stage centering procedure

- 4.4.1. Place a slide on the stage and focus on a particle with the 10X or higher magnification objective.
- 4.4.2. Locate a small particle and move it under the intersection of the crosslines.
- 4.4.3. Rotate the specimen 180 degrees, and if the particle does not stay under the crosslines, note the position.
- 4.4.4. Use the stage centering wrenches and move the stage so the particle is halfway to the intersection of the crosslines.
- 4.4.5. Move the slide so the particle is back under the intersection of the crosslines.
- 4.4.6. Rotate the stage, and the particle should stay under the crosslines. If the particle does not stay under the intersection of the crosslines, repeat steps until the stage is centered.

NOTE: Stage centering is not necessary on microscopes with a fixed stage.

4.5. Objective centering

- 4.5.1. Place a prepared slide on the stage and focus on a particle with the objective used to center the stage in the above procedure.
- 4.5.2. Locate a small particle and move it under the intersection of the crosslines.
- 4.5.3. Close the field diaphragm down and check that it is in good focus and centered.
- 4.5.4. Rotate the nosepiece to an objective having a different magnification and turn the stage 180 degrees monitoring the particle as above.
- 4.5.5. Adjust as was done when centering the stage, but this time use the centering wrenches in the nosepiece (not the stage centering screws) until the selected particle remains centered under the crosshairs when rotating the stage.
- 4.5.6. Follow the same procedure for each objective, if applicable.



ATF-LS-TE02 Setup and Use of the Microscope	ID: 1922 Revision: 6
Authority: Technical Leader	Page: 4 of 7
Original maintained by Quality Programs; copies are uncontrolled.	

4.6. Ocular Focus Adjustment

- 4.6.1. Verify the ocular with the crosslines and/or micrometer is in the right ocular tube and that the positioning pin on the ocular is inserted correctly in the ocular tube.
- 4.6.2. Block the light from the left ocular using a piece of paper or similar object.
- 4.6.3. Adjust the knurled ring on the right ocular and bring the crosslines and/or micrometer scale into good focus.
- 4.6.4. Focus on the specimen with the 40X objective. The specimen and the crosslines and/or micrometer should both be in sharp focus through the right ocular.
- 4.6.5. Block the light from the right ocular and view the specimen with the left ocular only.
- 4.6.6. Adjust the diopter adjustment ring on the left ocular to bring the particle into sharp focus.
- 4.6.7. Now the particle should be in good focus for both eyes.

4.7. Calculating the Ocular Scale Magnification Factor

- 4.7.1. The microscope's ocular scale is often used in a comparative manner, such as in comparing the number of ocular scale divisions in the width of two fibers. If a measurement is to be described in units other than ocular scale divisions, such as millimeters or micrometers, then a calibrated stage micrometer is used to calculate the ocular scale magnification factor. Once established, further performance checks of a microscope are not required unless the microscope has been moved or damaged.
- 4.7.2. If the stage micrometer becomes damaged, it shall be taken out of service and sent for a quality check by an external calibration lab. If all of the points on the stage micrometer are not certified/calibrated, then only the certified/calibrated points shall be used.
- 4.7.3. Usually for a microscope, the micrometer scale is 1 mm long divided into 100 divisions, so each division of the scale is 10 μm .
 - 4.7.3.1. The micrometer scale is placed on the stage and brought into good focus.



ATF-LS-TE02 Setup and Use of the Microscope	ID: 1922 Revision: 6
Authority: Technical Leader	Page: 5 of 7
Original maintained by Quality Programs; copies are uncontrolled.	

- 4.7.3.2. Move the micrometer scale so it is parallel to the ocular scale but slightly off-set. The ocular scale shall also be in good focus (see “Ocular focus Adjustment” above).
- 4.7.3.3 Use as much of the length of the two scales to obtain the greatest accuracy. For example, for the 40X objective the division lines for both scales overlap in such a manner that 80 ocular scale divisions overlap 20 stage scale divisions. Since each stage scale division represents 10 μm , the length is 200 μm . 80 ocular scale divisions divided into 200 μm equals 2.5 μm per ocular scale division.
- 4.7.3.4. This process shall be conducted for each objective.

NOTE: When the ocular scale is calculated, it shall be recorded in the logbook.

4.8. Alignment of the polarizer and the analyzer with ocular crosslines

- 4.8.1. Set the rotating analyzer to the “zero” mark.
- 4.8.2. Place a straight synthetic fiber on the stage and bring the object into good focus.
- 4.8.3. Move the slide so the fiber is directly under the intersection on the crosslines.
- 4.8.4. Insert the analyzer (cross the polars) and rotate the polarizer in the condenser so the field of view is as black as possible.
- 4.8.5. Rotate the fiber to extinction.
- 4.8.6. Uncross the polars and check to see if the fiber is parallel with the “East-West” crossline or the “North-South” crossline.
- 4.8.7. If not, carefully loosen the head of the microscope and rotate the head until the fiber is parallel to one of the crosslines. Re-tighten the head.
- 4.8.8. Cross the polars and check that the fiber is at extinction when parallel to the crossline. If not, repeat the steps.

5. Quality assurance and controls

- 5.1. Proper alignment of the microscope is completed upon initial receipt of the microscope. The microscope is readjusted or optimized as needed during use. See 4.2 above for modified Köhler illumination.



ATF-LS-TE02 Setup and Use of the Microscope	ID: 1922 Revision: 6
Authority: Technical Leader	Page: 6 of 7
Original maintained by Quality Programs; copies are uncontrolled.	

- 5.2. A color/light balance check shall be performed on the comparison microscope prior to use in casework.
 - 5.2.1. This is completed by checking the red, green, and blue reference fibers (F10.8, F10.126 and F10.195) and ensuring that a single fiber viewed on two slides appears similar in color and background.
 - 5.2.2. Readjusting for Köhler illumination/modified Köhler illumination as well as changing the light intensity may assist with balancing the microscope.
 - 5.2.3. Documentation of the check is recorded in the case record (e.g., “Color/light balance check completed”).
 - 5.2.4. The comparison microscope will be taken out of service if the color/light does not appear similar with the reference fibers.
- 5.3. Dust can be detrimental to microscopes and optical quality. When a microscope is not in use, it should be protected (covered). Stereomicroscopes should have their oculars covered minimally while other microscopes should be covered in their entirety. Never leave a tube or objective port open so that dust can get to the internal surfaces. Through proper set-up, regular maintenance and adjustments, the quality of this method is maintained.
- 5.4. In instances where the microscope is not functioning properly (e.g., artifacts are seen in the field of view, the field of view is dark) and cannot be corrected by an examiner, a qualified service technician shall be called and/or the microscope will be removed from service.
- 5.5. Microscopes should be cleaned, lubricated, and maintained periodically by a qualified service technician. The maintenance shall be documented (e.g., Logbook).
- 5.6. The calibrated micrometer shall be taken out of service and sent out for a quality check if damage occurs.

6. References

Manufacturer’s Instrument Manual

“Polarized Light Microscopy” McCrone, McCrone, and Delly (2001 or previous editions) McCrone Research Institute, Chicago, IL 60616



ATF-LS-TE02 Setup and Use of the Microscope	ID: 1922 Revision: 6
Authority: Technical Leader	Page: 7 of 7
Original maintained by Quality Programs; copies are uncontrolled.	

McCrone W. C., Particle Characterization by PLM: Part I No Polars, The Microscope, Vol. 30, No. 3, 1982, p185-196

McCrone W. C., Particle Characterization by PLM: Part II Single Polar, The Microscope, Vol. 30, No. 4, 1982, p315-331

McCrone W. C., Particle Characterization by PLM: Part III Crossed Polars, The Microscope, Vol. 31, No. 2, 1983, p187-206

SWGMAF Fiber Guidelines <https://www.asteetrace.org/subfiber>



ATF-LS-TE03-Use of the Microspectrophotometer	ID: 1923 Revision: 6
Authority: Technical Leader	Page: 1 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

1.1. This method describes the procedure for use of the Microspectrophotometer (MSP). MSPs are used to measure color characteristics in transmission, reflectance, or fluorescence of microscopic samples in the ultraviolet, visible, and near infrared regions. MSP is especially helpful when trying to distinguish between dyed samples having a similar color. The sample area is viewed directly, which allows precise targeting of the region to be spectrally analyzed. MSP is non-destructive and often requires little sample preparation.

1.2. Reference(s) to applicable OSAC Registry documents

1.2.1. ASTM E2808 Standard Guide for Microspectrophotometry in Forensic Paint Examinations

2. Instrumentation/Reagents

2.1. Specifics regarding the MSP instrumentation (manufacturer and model) and operating conditions shall be included on the data or on a separate parameter sheet that will be maintained in the case record. The current version of the software will be documented in the logbook.

2.2. Mounting media for transmission and fluorescence such as Permount, Cargille oils, Entellen, or glycerol.

3. Safety Considerations

3.1. Keep lamp housings a safe distance away from flammable objects. Make sure lamp housings are cool prior to placing cover over instrument.

3.2. Follow standard laboratory safety procedures.

4. Procedure or Analysis

4.1. Alignment

4.1.1. When using the MSP, the microscope shall be properly aligned and adjusted prior to taking any measurements to assure optimum performance. Consult work instructions or manufacturer's manuals for alignment procedures.



ATF-LS-TE03-Use of the Microspectrophotometer	ID: 1923 Revision: 6
Authority: Technical Leader	Page: 2 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

4.2. Sample preparation

4.2.1. Sampling and preparation will vary depending on the type of sample, the light sources and filters utilized, and prior testing conducted on the sample. Many samples to be run on the MSP will be mounted on glass microscope slides in a mounting medium from previous microscopical examinations. Analyzing these samples is acceptable; however, several things shall be taken into consideration:

- 4.2.1.1. For transmission, the sample shall be thin / translucent enough to transmit light.
- 4.2.1.2. For fluorescence, consideration shall be taken regarding the mounting media. Many common mounting media fluoresce which may interfere with the sample's intrinsic fluorescence.

4.3. Dark and Reference Scans

- 4.3.1. A Dark Scan is a measurement of the instrument void of any light. A Reference Scan is a measurement of the light transmitting/absorbing effect of all the components except for the sample of interest. The instrument is directed to take both during "Collect Dark & Reference".
- 4.3.2. The Dark and Reference Scans are needed for all types of samples and new Dark and Reference Scans are needed at minimum when introducing a new slide or substrate. The instrument conditions (e.g., objective, aperture size) shall be the same for the Dark and Reference Scans as they are for the sample (excluding fluorescence).
- 4.3.3. Transmission and Reflectance: When the sample is mounted on a glass microscope slide, it should be noted that microscope slides, cover slips, and mounting media are not optical grade components; therefore, if moving outside of the field of view, new Dark and Reference Scans should be taken. Generally, for this type of sample, the reference measurement will be taken on a blank area of the slide. For reflectance, a reference measurement should normally be taken on the substrate of the sample itself, if possible, or on an item having a similar reflectivity to the sample.
- 4.3.4. Fluorescence: The collection of the Dark and Reference Scans do not need to be repeated for different filters as it is only using the Dark Scan; the Reference Scan is not relevant.



ATF-LS-TE03-Use of the Microspectrophotometer	ID: 1923 Revision: 6
Authority: Technical Leader	Page: 3 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

4.4. Sample collection

- 4.4.1. Whether collecting spectra in transmission, reflectance, or fluorescence, be sure that the appropriate light sources and filters are in use. Optimize the system when needed by running programs, such as Autaset Optimize, and by collecting a new Dark and Reference Scan as described above. The instrument conditions (e.g., objective, aperture size) shall be the same for the Dark and Reference Scan as they are for the sample (excluding fluorescence). The parameters used to collect the sample will vary depending on the properties of the sample. For specific instructions on collecting sample spectra, refer to the work instructions or manufacturer's manual.

4.5. Sampling

- 4.5.1. In most instances, multiple spectra will be collected of each sample to determine the range of variation. The number of spectra needed to determine this range will vary from one material to another (e.g., synthetic fiber dyes tend to be very uniform, so fewer spectra would be required to determine this variation than would be required for a natural fiber which generally absorbs dye in different amounts along the length of the fiber). The range of variation shall be considered when determining where to take the spectra from (e.g., sampling from areas that vary in properties such as color and shade).
- 4.5.2. For paint samples, E2808¹ recommends that at least five spectra are collected from non-effect paint films and a larger number for paints with effect pigments. The number is adjusted to capture the variation present within the sample. Small sample size or poor sample conditions may preclude this.

4.6. Display

- 4.6.1. There are many different and acceptable ways to display the spectra obtained from the MSP.
- 4.6.2. When comparing a questioned and a known sample, a display method shall be utilized that will allow the technical reviewer to see that the questioned sample falls within a range of variation seen in the known or that demonstrate the exclusionary differences. This may be done through mathematics (standard deviation and mean) or by simply displaying the questioned spectrum and the known spectra (spectral overlay), which is a recognized method for comparing data where the presence or absence of peaks, peak shapes, and relative intensities

¹ ASTM E2808 Standard Guide for Microspectrophotometry in Forensic Paint Analysis



ATF-LS-TE03-Use of the Microspectrophotometer	ID: 1923 Revision: 6
Authority: Technical Leader	Page: 4 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

are all considered. It shall be left to the discretion of the examiner to choose which display method is most appropriate for their case.

- 4.6.3. Transmission spectra can be displayed in % Transmission or Absorbance and Reflectance spectra can be displayed as % Reflectance or Absorbance. Absorbance data is linear regarding concentration, so this type of display may provide more information on relative concentrations.

4.7. Spectral Comparison and Interpretation

- 4.7.1. MSP spectral comparisons are conducted between spectra collected using similar sample preparation methods and similar instrumental parameters.
- 4.7.2. Comparisons include examination of peak shape, minima, maxima, inflection points, troughs, shoulders, relative peak intensities, and the curves or slopes between peaks.
- 4.7.3. When assessing differences between spectra, consider sample limitations (e.g., sample size, dirty samples, thickness) and instrument limitations (e.g., aperture).
- 4.7.4. Samples are considered distinguishable when exclusionary differences are observed. An exclusionary difference is defined as a difference in one or more characteristics between items that is sufficient to determine that the compared items did not originate from the same source, are not the same source, or do not share the same composition or classification². Exclusionary differences in spectral comparisons: (1) are outside the variability of spectra originating from the same source; and (2) cannot be explained by considerations such as sample heterogeneity, contamination, different sample conditions, or different sample histories.
- 4.7.5. Samples are considered indistinguishable when no exclusionary differences are observed between compared spectral features.

5. Quality Assurance and Controls

- 5.1. Proper alignment of the microscope was completed when the instrument was installed. System alignment is checked prior to taking any measurements and is readjusted as needed during the examination.

² OSAC Preferred Terms. Available online [accessed October 2022]
https://www.nist.gov/system/files/documents/2022/08/10/OSAC%20Preferred%20Terms_August%202022.pdf



ATF-LS-TE03-Use of the Microspectrophotometer	ID: 1923 Revision: 6
Authority: Technical Leader	Page: 5 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

5.2. Performance check

5.2.1. Performance checks shall be performed each day prior to use in casework. Consult work instructions or manufacturer's manuals on how to complete the performance checks. Performance checks for each lamp used will include the following:

5.2.1.1. Wavelength check utilizing Holmium Oxide and Didymium glass filters.

5.2.1.2. Photometric check utilizing ND 0.1, ND 0.5, and ND 1.0 neutral density filters

5.3. The calibration standards (glass and neutral density filters) are traceable to Standard Reference Materials issued by NIST. Filters shall be recertified upon the manufacturer's expiration date.

5.4. The alignment check, performance check, and calibration standard certificates are documented in the instrument logbook.

5.5. Validation

5.5.1. MSP is a well-known and scientifically accepted method for the identification, analysis, and comparison of many types of trace evidence. Relevant examples of the broad nature of the method and related literature can be found in Section 6 (References).

6. References

Operations Manual for the Microspectrophotometer

Biermann TW, Wiggins KG. "Colour Analysis of Fibres" in Forensic Examination of Fibres, 3rd ed., Robertson J, Roux C and Wiggins KG, ed(s), Taylor & Francis Group LLC: Boca Raton, FL, 2018.

Eyring MB, Visible Microscopical Spectrophotometry in the Forensic Sciences, Forensic Science Handbook, 2nd edition, Vol 1, Saferstein R, Ed., Prentice-Hall: Upper Saddle River, NJ 2002.

Stoecklein W. "The role of colour and microscopic techniques for the characterization of paint fragments" in Forensic Examination of Glass and Paint, Caddy B, Ed., Taylor and Francis: New York, NY 2001.



ATF-LS-TE03-Use of the Microspectrophotometer	ID: 1923 Revision: 6
Authority: Technical Leader	Page: 6 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

SWGMA T “Ultraviolet-Visible Spectroscopy of Textile Fibers Chapter” (2011 Update).
Available online: <https://www.astetrace.org/static/images/pdf/03%20UV-VIS%20Spectroscopy%20of%20Textile%20Fibers%20Chapter%20%282011%20Update%29.pdf>



ATF-LS-TE-04-Pyrolysis-Gas Chromatography/Mass Spectrometry (PyGC-MS)	ID: 1924 Revision: 4
Authority: Technical Leader	Page: 1 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

1. Introduction

1.1 Pyrolysis is a technique used to break chemical bonds of molecules by the use of thermal energy only. Analytical pyrolysis is a technique to study molecules by observing their behavior during pyrolysis and the resulting molecular fragments.

1.2 Pyrolysis breaks large molecules in the pyrolysis chamber within a short period of time into smaller fragments, which are called pyrolysates. During pyrolysis, helium gas is constantly flowing through the pyrolysis chamber providing an inert atmosphere. This constant flow of helium carries the pyrolysates from the pyrolysis chamber into the GC column for separation and then the GC separated pyrolysates are sorted and detected by MS. A pyrogram (reconstructed total ion chromatogram) is acquired which represents the separated pyrolysates.

2. Instrumentation/Reagents

2.1 Gas Chromatograph: Capable of using capillary columns and being interfaced to a mass spectrometer.

2.2 Mass Selective Detector with EI Source: Capable of scanning between 20 and 600m/z with unit resolution or better, with continuous data output.

2.3 Computerized data station: Capable of storing chromatographic and mass spectral data from sample runs; Capable of performing, either through its operating system or by user programming, various data handling functions, including input and storage of sample data files, searching data files for selected compounds, and qualitative and semi-quantitative compound analysis.

2.4 Autosampler: Pyrolysis autosampler, accessories, and software

2.5 Carrier gas: Helium, 99.99% (high purity)

2.6 Sample holder: vertical quartz tube or alloyed metal cups

2.7 Commercially available polymers (e.g., polystyrene, polyethylene, Kraton, or other suitable polymer products).

2.8 Cleaning apparatus for sample holders (e.g., aluminum block, small butane torch, sample cup inspector)

2.9 Stereomicroscope and glass microscope slides



ATF-LS-TE-04-Pyrolysis-Gas Chromatography/Mass Spectrometry (PyGC-MS)	ID: 1924 Revision: 4
Authority: Technical Leader	Page: 2 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

2.10 Scalpel with blades and other appropriate sampling tools

2.11 Analytical microbalance

3. Safety Considerations

3.1 All gas cylinders must be properly secured, and pressure regulators should be inspected whenever cylinders are replaced.

3.2 Precautions need to be taken whenever working with chemicals which could pose potential health hazards.

3.3 Avoid direct contact with any of the heating elements associated with the pyrolyzer to include the heating coil and the furnace of the vertical micro-furnace pyrolyzer. These heating elements can be extremely hot and can cause burns.

4. Procedure or Analysis

4.1. Sample Preparation

4.1.1. The appropriate container will be used for analysis (e.g., vertical quartz tubes or an alloyed metal cup.)

4.1.2. Liquid samples

4.1.2.1. A liquid sample can be directly dispensed into the center of a metal alloy cup or vertical quartz tube. A suitable sample size is one that provides sufficient signal to identify the characteristic components.

4.1.3. Solid Samples

4.1.3.1. Sample size is sample dependent on instrument sensitivity and the chemical composition of the material; however, similar sample sizes should be used for all samples being compared. It is critical that all tools for sample preparation are clean; otherwise, contamination could lead to inaccurate results. The ideal positioning of a sample is in the center of the alloyed metal cup for the micro-furnace pyrolyzer or vertical quartz tube.

4.2 Data analysis and interpretation

4.2.1 The following will be used as a guide in determining the acceptability of the data.



ATF-LS-TE-04-Pyrolysis-Gas Chromatography/Mass Spectrometry (PyGC-MS)	ID: 1924 Revision: 4
Authority: Technical Leader	Page: 3 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

4.2.2 Comparative Analysis - Comparison of an unknown sample to a known sample(s): Pattern comparisons are done using pattern recognition techniques and mass spectral identification techniques when deemed necessary. For ensuring the best results, it is very important to have samples of the same size and geometry. Pyrograms can be compared on screen, side-by-side, or using overlays. Documentation of pattern comparisons shall be included in the case jacket. Factors that should be considered include the peak shape, retention time, and the relative peak intensity.

4.2.2.1 The peak shape (symmetry, width, etc.) should display reasonable agreement between the samples.

4.2.2.2 The retention time and mass spectral data should have reasonable agreement with each other. The retention time of peaks being compared in two or more programs should be within $\pm 2\%$ of each other.

4.2.2.3 The relative intensities of the peaks should display reasonable agreement between the comparison samples. Factors affecting peak intensities should be considered, which include sample size, heterogeneity of the sample, sampling technique, and the reproducibility of the pyrolysis process.

4.2.3 Identification analysis: Identification of a known or unknown sample shall be made by running a reference standard or in some circumstances, by comparing the sample to a standard reference library.

4.2.4 The presence of additional peaks should be further examined to assess if a possible source can be determined. Additional peaks could be inherent differences between samples, from extraneous material adhering to a sample, or system peaks, such as siloxanes.

4.2.4.1 If extraneous material is the likely source of the additional peaks, a new sample should be prepared and analyzed.

4.2.4.2 If it is suspected that the additional peaks are due to inherent differences, the heterogeneity of a sample can be assessed through the analysis of replicate samples.

4.2.5 Samples are considered distinguishable if one or more exclusionary difference is observed. The definition of an exclusionary difference is “a difference in a



ATF-LS-TE-04-Pyrolysis-Gas Chromatography/Mass Spectrometry (PyGC-MS)	ID: 1924 Revision: 4
Authority: Technical Leader	Page: 4 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

feature or property between compared items (e.g., pyrograms) that is substantial enough to conclude that they did not originate from the same source”.

4.2.6 Instrument operating parameters shall be included in the case record when the PyGC-MS is used in casework.

4.3 Limitations

4.3.1 PyGC-MS is a destructive analytical technique.

4.3.2 PyGC-MS is limited to identifying the organic materials present in a sample. No inorganic information can be obtained from this technique.

4.3.3 Sample size and/or condition may preclude examination by this technique.

4.3.4 The analysis of combined layers or items will hinder the ability to differentiate between the individual layers/items.

5. Quality Assurance and Controls

5.1. Tune and Performance Check

5.1.1. The instrument will be tuned within one week prior to casework analysis. The tune report shall be examined to ensure that the appropriate parameters are within their normal expected range specified by the manufacturer and initialed by the examiner performing the tune. Documentation that the values were verified as meeting manufacturer's specification will be maintained in the instrument logbook. The tune reports are maintained near the instrument. The tune date(s) will be recorded in the case file.

5.2. Quality Control

5.2.1. A suitable polymer standard (e.g., polystyrene, Kraton) will be run at the start and end of each casework related sequence. If a break in analysis occurs, an intermittent standard will be run for each break that occurs. The data shall be assessed each time the instrument is run to ensure operating performance, mass assignment, and overall good chromatography. A different suitable polymer standard will be run within at least 30 days of sample analysis to assess monthly operating performance, column selectivity, and continued integrity of the system (e.g., high-density polyethylene). Refer to the appropriate work instructions for monitored criteria (e.g., retention time, baseline separation), “pass/fail” criteria, and documentation requirements.



ATF-LS-TE-04-Pyrolysis-Gas Chromatography/Mass Spectrometry (PyGC-MS)	ID: 1924 Revision: 4
Authority: Technical Leader	Page: 5 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

- 5.2.2. If the standard indicates poor chromatography, the error shall be corrected and documented in the logbook. Refer to instrument manual for suggested maintenance/troubleshooting techniques and/or contact the primary operator for assistance.
- 5.2.3. When maintenance is performed that affects chromatography, a quality control standard will be analyzed, and the appropriate monitored criteria will be recorded to ensure criteria are met. If changes outside the normal expected range occur in the tune and/or standards, the error shall be corrected and documented in the logbook. Refer to the instrument manual for suggested maintenance/troubleshooting techniques. All maintenance will be documented in the instrument logbook.

5.3. Material Control and System Blank

- 5.3.1. A material control (e.g., stainless steel cup, stainless steel cup with solvent, quartz tube) will be evaluated prior to casework samples to show that the material(s) used for sample preparation are free of contamination.
- 5.3.2. A system blank (e.g., stainless steel sample cup, quartz tube, no sample cup, or no quartz tube) will be run in between samples to demonstrate carryover is not occurring.
- 5.3.2.1. Carryover typically signifies that an overloaded sample was introduced into the system, leading to an atypical blank where extraneous peaks are present.
- 5.3.2.2. The presence of carryover may require running additional blanks to diminish the effects of an overloaded sample.
- 5.3.2.3. In addition to running additional blanks, adjusting the sample size to provide an adequate signal is advisable to help prevent the reoccurrence of carryover.
- 5.3.2. A blank demonstrates the lack of contamination of analytes of interest. A blank should not display any chromatographic peaks greater than the CO₂ response. If extraneous peaks are present, an attempt will be made to determine the source of these peaks and will be documented in the case notes, otherwise, the affected exhibits will be reanalyzed.



ATF-LS-TE-04-Pyrolysis-Gas Chromatography/Mass Spectrometry (PyGC-MS)	ID: 1924 Revision: 4
Authority: Technical Leader	Page: 6 of 6
Original maintained by Quality Programs; copies are uncontrolled.	

5.3.3 Through regular quality control checks of known standards and upkeep of instrument logbooks the quality of the PyGC-MS method is assured.

6. References

6.1 ASTM International Standards

ASTM E1610 Standard Guide for Forensic Paint Analysis and Comparison
ASTM E3260 Standard Guide for Forensic Examination and Comparison of Pressure Sensitive Tapes
ASTM E3296 Standard Guide for Using Pyrolysis Gas Chromatography and Pyrolysis Gas Chromatography-Mass Spectrometry in Forensic Polymer Examinations

6.2 Instrument user, maintenance, and troubleshooting manual(s) for GC-MS, pyrolyzers, and associated accessories.

CDS Analytical, Inc., Pyrolysis Application Review

Frontier Laboratories LTC Operation Manual

FBI Performance Monitoring Protocol for the Pyrolysis-GC/MS

6.4 Other

Irwin, William J., Analytical Pyrolysis-A Comprehensive Guide, Chromatographic Sciences Series, Vol. 22, Marcel Dekker, Inc., New York, 1982.

Saferstein, R. "Forensic Analytical Pyrolysis", Proceedings of the International Symposium on the Analysis and Identification of Polymers 1984, pp 9-18.

Wampler, Thomas P, Applied Pyrolysis Handbook, Marcel Dekker, Inc., New York, 1995.

Wampler, T. P. and Levy, E. J., "Reproducibility in Pyrolysis, Recent Developments," Journal of Analytical and Applied Pyrolysis, 12, 1987, pp 75-82.



ATF-LS-TE07 Handheld Raman Spectrometer	ID: 1932 Revision: 7
Authority: Technical Leader	Page: 1 of 2
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

1.1. Raman spectroscopy is a non-destructive analytical technique used for identification of unknown chemicals. The Raman spectrum can provide enough characteristics to specifically identify a substance, and in some cases a mixture of substances. Reference spectra of thousands of materials are available for comparison and identification of unknowns.

2. Instrumentation/Reagents

2.1. A Raman spectrometer equipped with a library of standards

3. Safety Considerations

3.1 All users should be properly trained on the safe operation of the instrument.

3.2 Raman relies on the use of a laser. Laser-related safety considerations:

3.2.1 Eye hazard – maintain at least 19 inches of distance between the laser and your eyes. Never look into the end of the probe.

3.2.2 Localized heating – the energy of the laser can cause localized heating of dark materials and some substrates (e.g. coffee filters). Avoid analysis of dark materials, or powders where dark flecks are present. Ensure the focal point of the laser is aligned with the analyte (e.g. not hitting paper under a pile).

3.3 Potentially energetic materials, such as suspected explosives, should be analyzed with the following precautions:

3.3.1 Scan delay should be used, and the user should move a safe distance from the instrument while the laser is on.

3.3.2 Run vials without a cap

3.3.3 Isolate a small amount of material from the bulk where possible

4. Procedure or Analysis

4.1. Conduct a self-test or verify the instrument has passed its self-test in the preceding 30 days.



ATF-LS-TE07 Handheld Raman Spectrometer	ID: 1932 Revision: 7
Authority: Technical Leader	Page: 2 of 2
Original maintained by Quality Programs; copies are uncontrolled.	

4.2. Testing and sample preparation will vary depending on the sample to be analyzed.

4.3. Ensure the focal point of the laser is aligned with the area to be sampled.

4.4. Review the spectral data as compared to the library results.

5. Quality Assurance and Controls

5.1. Performance Verification: The instrument must pass the manufacturer's Self-Test using the polystyrene standard provided by the vendor (or equivalent substitute) within 30 days prior to use. The results of the Self-Test will be documented in the log book.

6. References

Bartick, E.G., Merrill, R.A., & Mount, K.H. (2001). Analysis of a Suspect Explosive Component: Hydrogen Peroxide in Hair Coloring Developer. Forensic Science Communications, 3(4).

Matthews, R.; Longworth, T.; Ong, K.; Zhu, L.; Brown, C.; Knopp, K. Testing of Ahura's Firstdefender Handheld Chemical Identifier Against Toxic Industrial Chemicals; Edgewood Chemical Biological Center, US Army Research, Development, and Engineering Command: Aberdeen Proving Ground, 2006.

Matthews, R.; Ong, K.; Brown, C.; Zhu, L.; Knopp, K. Evaluation of Ahura's First Defender Handheld Chemical Identifier; Edgewood Chemical Biological Center, US Army Research, Development, and Engineering Command: Aberdeen Proving Ground, 2006.

Moore, D., & Lee, K. (2007). Raman spectroscopy as a tool for long-term energetic material stability studies. Journal of Raman Spectroscopy, 38(9), 1221-1224.



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 1 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

1.1. The forensic hair examiner can be requested to analyze a questioned sample for the purpose of identifying it as a hair, if it came from an animal or a human being. If the hair is from an animal, species identification may be attempted. If from a human, the somatic origin (body area) of the hair may be determined by general morphology. A human hair may also be associated to a particular ancestry group based on established models for each group. Forensic hair examiners differentiate between hairs of European ancestry, Asian ancestry, and African ancestry origin, all of which exhibit microscopic characteristics that distinguish one ancestral group from another. Also, hairs may be evaluated to determine if further microscopical comparisons and/or DNA analysis can be conducted.

2. Instrumentation/Reagents

2.1. Sticky sided collecting materials such as tape or Post-it notes

2.2. Forceps

2.3. Containers such as glassine envelopes, plastic bags or vials

2.4. Illuminated magnifier

2.5. Transparent securing substrates such as slides or sheet protectors

2.6. Vacuum, with clean filter attachments for collecting hairs

2.7. Glass microscope slides

2.8. Glass cover-slips

2.9. Mounting medium

2.10. Stereomicroscope

2.11. Transmitted light microscope

2.12. Miscellaneous laboratory supplies or equipment

3. Safety Considerations



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 2 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

- 3.1. The examiner should follow all the biohazard procedures and use universal safety precautions.
- 3.2. Precautions need to be taken whenever working with chemicals which could pose potential health hazards.

4. Procedure or Analysis

4.1. Recovery of hairs

4.1.1 Purpose

Generally speaking, submitting the article or articles of evidence to the laboratory for the examiner to process is the best approach to the recovery of hairs. There are instances where this is not practical or possible, such as recovering hairs from wall-to-wall carpeting, a large piece of furniture, or a vehicle. In these instances, the recovery of hairs may be accomplished at the scene by any of the following methods and submitted for examination. Hairs may be recovered by manually removing them from an item, or the item may be taped, scraped, or vacuumed in an effort to remove hairs of interest.

4.1.2 Minimum standards and controls

4.1.2.1 The examiner must clean the examination area and change the examination paper between victim and suspect or scene exhibits.

4.1.2.2 The examiner must change gloves and clean their tools between examining the evidence from different individuals or locations. Use separate laboratory coats during the collection of the known and questioned items.

4.1.2.3 Items from different individuals and different locations are separated in time and/or space. At no time should questioned items and known items be open at the same time in the same area for recovery of trace evidence.

4.1.3 Analytical procedure

4.1.3.1 Document the condition of the submitted items.

4.1.3.2 Examine each item of evidence visually or with the aid of an illuminated magnifier, or low powered microscope.



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 3 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

- 4.1.3.3 If the item being examined contains hairs that are readily visible, collect them. As hairs are collected, they should be secured and/or preserved in an appropriate manner.
- 4.1.3.4 Care should be taken to avoid the loss of any hairs, especially when repositioning bulky items.
- 4.1.3.5 Adhesive tapes and/or other adhesive devices (e.g. “Post-it Notes”, lint rollers, etc) may be used to recover hairs. The adhesive surface is placed on the item being examined and then pulled away. The tape may then be placed on a clean sheet of plastic (e.g. sheet protector) for further examination and storage.
- 4.1.3.6 Other collection methods may be used including vacuuming and scraping. If scraping is necessary, the item to be examined is suspended above the examination surface and very gently scraped with a spatula. Scraping in a downward direction allows surface hairs to fall onto the examination surface for collection. If vacuuming is used then separate filters should be used for different areas.
- 4.1.3.7 When recovering hairs from tape present on submitted items, it is important to remember that exposed areas of the tape may contain environmental (scene) hairs that may be of no probative value, while hairs found under the adhesive may be extremely valuable. Latent print considerations of these tape pieces are paramount as well as other trace evidence (see “Pressure Sensitive Tape Protocol”). Multiple layers of tape should be separated layer by layer and examined for any hairs in protected areas or other evidence that could have originated from the environment in which the item was manufactured. This may be done by the latent print examiner, the explosives chemist, or the trace evidence examiner. Hairs found in the protected areas of the tape are removed with clean forceps for examination. The exposed tape adhesive may be placed on a clean non-porous surface for transfer to latent prints.

4.2 Hair examination and analysis

4.2.1 Purpose

The purpose of hair examinations and analyses is to identify hairs as to their type (human or animal), identify species or ancestry characteristics, and identify somatic origin.

4.2.2 Minimum standards and controls



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 4 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

A reference collection of hairs may be useful to the examiner when determining if hairs are animal or human, or for identifying species, ancestry characteristics, or somatic origin.

4.2.3 Sample selection

Groups of questions hairs cannot be assumed to be from the same individual / body area/ animal, sample selection will be utilized when reporting probative microscopical hair examinations. Each hair will be examined independently from all others and results in reports should reflect this.

4.2.4 Analytical procedure

Observe the physical properties of the mounted hairs utilizing transmitted light microscope having a magnification range of at least 100X to 400X. When possible, classify the hair as animal or human, identify species or ancestral characteristics, and identify somatic origin based on the characteristics noted.

4.2.4.1 The following microscopic characteristics are commonly used to determine if a hair is animal or human:

4.2.4.1.1 Human hairs:

4.2.4.1.1.1 Medulla is generally amorphous in appearance and the width is generally less than one-third the overall diameter of the hair shaft.

4.2.4.1.1.2 Scales are not usually pronounced and the structure is imbricate.

4.2.4.1.1.3 Pigment granules are usually distributed toward the cuticle (with the exception of naturally red hair which is often distributed toward the medulla)

4.2.4.1.1.4 Generally, the color and pigmentation is consistent throughout the length of the hair shaft.

4.2.4.1.1.5 The root is commonly club-shaped or stretched.

4.2.4.1.2 Animal hairs:

4.2.4.1.2.1 Medulla is frequently continuous and structured. The width is usually greater than one-third the overall diameter of the hair shaft.



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 5 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

- 4.2.4.1.2.2 Scales are often pronounced, and the structure of the scales can be coronal, spinous, or imbricate.
 - 4.2.4.1.2.3 Pigment granules are usually distributed toward the medulla. Radical changes in color along the length of the hair shaft, called banding, is common.
 - 4.2.4.1.2.4 The shape of the root is highly variable.
- 4.2.4.2 The following microscopic characteristics are commonly used to determine the ancestral origin of a human hair:
- 4.2.4.1.1 European Ancestry:
 - 4.2.4.1.1.1 Shaft diameter is moderate with minimal variation (mean diameter of human head hairs – 80um)
 - 4.2.4.1.1.2 Pigment granules are sparse to moderately dense with fairly even distribution.
 - 4.2.4.1.1.3 Cross-sectional shape is oval.
 - 4.2.4.1.2 African Ancestry:
 - 4.2.4.1.2.1 Shaft diameter is moderate to fine with considerable variation.
 - 4.2.4.1.2.2 Pigment granules are densely distributed (hair shaft may be opaque) and arranged in prominent clumps or streaks.
 - 4.2.4.1.2.3 Shaft has prominent twist and curl.
 - 4.2.4.1.2.4 Cross-sectional shape is flattened.
 - 4.2.4.1.3 Asian Ancestry:
 - 4.2.4.1.3.1 Shaft diameter is coarse and usually with little or no variation.
 - 4.2.4.1.3.2 Pigment granules are densely distributed and often arranged in large patchy areas.



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 6 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

4.2.4.1.3.3 Medulla is prominent (often broad and continuous).

4.2.4.1.3.4 Cuticle is thick with typically clear cuticular margin.

4.2.4.1.3.5 Cross-sectional shape is round

4.2.4.1.4 Mixed Ancestral Hairs:

4.2.4.2.4.1 Hairs exhibiting characteristics common to more than one ancestral group.

4.2.4.2 The following microscopic characteristics are commonly used to determine the somatic origin of a human hair:

4.2.4.2.1 Head hairs:

4.2.4.2.1.1 Long with moderate shaft diameter variation.

4.2.4.2.1.2 Medulla absent to continuous and relatively narrow when compared to the structure of hairs from other body areas.

4.2.4.2.1.3 Cut, abraded, split or broken tips.

4.2.4.2.1.4 May show artificial treatment or solar bleaching.

4.2.4.2.1.5 Soft texture, pliable.

4.2.4.2.2 Pubic hairs:

4.2.4.2.2.1 Shaft diameter course with wide variations and buckling.

4.2.4.2.2.2 Medulla relatively broad and usually continuous when present.

4.2.4.2.2.3 Root frequently with a follicular tag.

4.2.4.2.2.4 Tip usually tapered, rounded, or abraded.

4.2.4.2.2.5 Stiff texture, wiry.

4.2.4.2.3 Limb hairs:



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 7 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

4.2.4.2.3.1 Diameter fine with little variation. Gross appearance of hair is arc-like in shape.

4.2.4.2.3.2 Medulla is discontinuous to trace with a granular appearance.

4.2.4.2.3.3 Tips usually taper and are often blunt and abraded. Scale ends are commonly rounded due to wear.

4.2.4.2.3.4 Soft texture.

4.2.4.2.4 Facial hairs:

4.2.4.2.4.1 Diameter very coarse with irregular or triangular cross-sectional shape.

4.2.4.2.4.2 Medulla very broad and continuous may be doubled.

4.2.4.2.5 Chest hairs:

4.2.4.2.5.1 Shaft diameter moderate and variable.

4.2.4.2.5.2 Tip often darker in color, long and fine, arc-like.

4.2.4.2.5.3 Medulla may be granular.

4.2.4.2.5.4 Stiff texture.

4.2.4.2.6 Axillary or underarm hairs:

4.2.4.2.6.1 Resemble pubic hairs in general appearance, but less wiry.

4.2.4.2.6.2 Medullary appearance similar to limb hairs.

4.2.4.2.6.3 Diameter moderate and variable with less buckling than pubic hairs.

4.2.4.2.6.4 Tips long and fine, frequently with a bleached appearance.

4.2.4.2.7 Other hairs:

4.2.4.2.7.1 Eyebrow: Stubby, some diameter fluctuation, saber-like in



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 8 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

appearance.

4.2.4.2.7.2 Eyelash: Short, stubby with little shaft diameter fluctuation, saber-like in appearance.

4.2.4.2.7.3 Trunk: A combination of features of limb and pubic hairs, a transitional hair.

4.2.4.2.7.4 Fringy: Hairs in transitional areas of the body may include characteristics from two areas. For instance the nape of the neck often contains fine hairs similar to head and body hairs.

4.2.5 Screening hairs for DNA analysis

4.2.5.1 Purpose

Recovered hairs may be screened to determine if they are suitable candidates for DNA analysis. If known head or pubic hairs are submitted and meaningful macroscopic/microscopic differences exist between known and unknown hairs, no further analysis may be necessary.

4.2.6 Minimum standards and controls

4.2.6.1 The examiner performing the examination must have sufficient training and knowledge for human hair screening for DNA analysis.

4.2.6.2 A transmitted light microscope and/or comparison microscope having high magnification range is required.

4.2.6.3 Generally, destructive testing such as DNA analysis is performed after all non-destructive examinations are completed.

4.2.7 Sample selection

Each hair will be examined independently from all others and results in reports should reflect this. It is left to the discretion of the hair examiner to determine the hairs which are most suitable for DNA analysis. Reports should reflect how many or which hairs were selected for additional DNA examinations.

4.2.8 Analytical procedure

4.2.8.1 Human hairs determined to be probative should be examined further microscopically to assess them for future microscopical and/or DNA examinations.



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 9 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

4.2.8.2 Certain somatic regions (e.g., head, pubic region) are generally considered suitable for microscopical comparisons though facial hairs also may be compared. The ATF Laboratories do not conduct hair comparisons; however, these hairs may be sent to another laboratory for this type of testing.

4.2.8.2.1 When the somatic origin of head, facial, or pubic region has been determined, it can be reported out that the hair(s) “are” suitable for microscopical comparison.

4.2.8.2.2 If somatic origin has not been determined, it can be reported out that the hair(s) “may” be suitable for microscopical comparison.

4.2.8.3 If root tissue is present on the hair in question, or if the hair has an anagen or catagen root, the hair is suitable for nuclear DNA analysis. If no root tissue is present, hairs may be selected for mitochondrial DNA analysis. The ATF Laboratories do not conduct mitochondrial DNA examination; however, these hairs may be sent to another laboratory for this type of testing.

4.2.8.4 Photographing the root and measuring the length of the hair prior to DNA analysis is recommended.

4.2.8.5 Hairs selected for additional analysis can be removed from the glass slides by a hair examiner. If permanently mounted, this may be done by punching a hole in the coverslip using a scribe, placing a drop of xylene or other suitable solvent in the hole to loosen the mounting media, and removing the hair with tweezers. If using a non-permanent mounting media, the coverslip may simply be lifted and the hair removed. The hair should be cleaned in a solvent such as xylene and then with water. The hair may then be placed in a bullet tube, or on a post-it note for transfer to the DNA unit. If placed on a post-it note, it is good practice to identify the root end. If the hairs are to be released to an external agency for analysis not performed at the ATF, the examiner should check with that agency for submission requirements.

5. Quality Assurance and Controls

5.1 Through proper training, competency testing, and proficiency testing of hair examiners as well as the use of high-quality microscopes which are cleaned and maintained appropriately, the quality of this method is maintained.



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 10 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

5.2 Validation

The techniques described above for hair examination are well known and scientifically accepted in the forensic science community and in private industry. Relevant examples of related literature can be found in Section 6 (References).

6 References

6.1 ASTM International Standards

6.1.1 E1459 Standard Guide for Physical Evidence Labeling and Related Documentation

6.1.2 E1492 Standard Practice for Receiving, Documenting, Storing and Retrieving Evidence in a Forensic Science Laboratory

6.2 Scientific Working Group for Materials (SWGMAT) Documents available at:
www.astetrace.org

6.2.1 Forensic Hair Examinations Guidelines

6.3 Other

6.3.1 Bisbing R. The Forensic Identification and Association of Human Hair. In: The Forensic Science Handbook, Volume 1, 2nd edition, Saferstein R, Ed. Upper Saddle River, NJ: Pearson Education, 2002.

6.3.2 Deedrick D, Koch S. Microscopy of Hair Part 1: A Practical Guide and Manual for Human Hairs. Forensic Science Communications, Vol 6, No.1, 2004.

6.3.3 Deedrick D, Koch S. Microscopy of Hair Part 2: A Practical Guide and Manual for Animal Hairs. Forensic Science Communications, Vol 6, No. 3, 2004.

6.3.4 Linch C, Smith S, Prahlow J. Evaluation of the Human Hair Root for DNA Typing Subsequent to Microscopic Comparison. J of For Sci, Vol 43 (2), pp 305-314, 1998.

6.3.5 Oien, CT. Forensic Hair Comparison: Background Information for Interpretation. Forensic Science Communications, Vol 1, No. 2, 2009.



ATF-LS-TE09 – Examination and Analysis of Hair Evidence	ID: 1927 Revision: 7
Authority: Technical Leader	Page: 11 of 11
Original maintained by Quality Programs; copies are uncontrolled.	

- 6.3.6 *Ogle R, Fox M. Atlas of Human Hair – Microscopic Characteristics. Boca Raton, FL: CRC Press. 1999.*
- 6.3.7 *Petraco N, Fraas C, Callery F, DeForest P. The Morphology and Evidential Significance of Human Hair Roots, J of For Sci, Vol 33 (1), pp 68-76, 1988.*
- 6.3.8 *Robertson J. Forensic Examination of Hair, London: Taylor and Francis, 1999.*



ATF-LS-TE10 Examination of Physical Fits	ID: 1928 Revision: 6
Authority: Technical Leader	Page: 1 of 3
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

1.1. To compare portions of pipes, tools, tapes, glass, fabrics, papers, and other items of evidence to determine whether those portions were once a part of or have been separated from, a particular source. This is done through a comparison of fractures and other surface features. If meaningful alignment of random characteristics can be established, an association can be made between two or more fragments/pieces and will demonstrate they were once joined together to form a single object.

2. Instrumentation/Reagents

2.1. Stereo and comparison microscope(s)

2.2. Micrometers, calipers, rulers

2.3. Casting media

2.4. Photographic equipment

3. Safety Considerations

3.1. Use appropriate personal protective equipment (glasses, gloves, lab coat).

3.2. Care shall be taken when handling exhibits with sharp edges.

4. Procedure or Analysis

4.1. Examine physical properties of item(s) to be compared (e.g., color, material type, dimensions, surface features). The questioned item shall be evaluated prior to the examination of the known item.

4.2. The separation method (e.g., cut, torn) can influence the features of a physical fit examination, however, specific damage assessment is outside the scope of this document.

4.3. Evaluate and compare class characteristics. When exclusionary differences are observed at any point during the examination, no further examinations are required.



ATF-LS-TE10 Examination of Physical Fits	ID: 1928 Revision: 6
Authority: Technical Leader	Page: 2 of 3
Original maintained by Quality Programs; copies are uncontrolled.	

4.4. Evaluate the shape of separation and check for any surface features that may be continuous on both sides of the separation. The elasticity of the object shall be taken into consideration especially in areas where the stretching due to separation may cause distortion in the physical fit.

4.5. If the item is of suitable thickness, examine the surface of the face of the separation to determine if the edge features correspond.

4.6. If the class characteristics of the separated pieces are compatible and if the pieces fit together in at least one of the following individualizing characteristics, it can be determined that the two items were at one time joined together to form a single continuous piece:

4.6.1. Along an irregular edge-to-edge border like a jigsaw puzzle matched over a reasonable length.

4.6.2. Continuous surface markings or internal features.

4.6.3. Three-dimensional fit

5. Quality Assurance and Controls

5.1. Performance checks and calibrations

Microscopes and/or micrometer/measuring devices shall be properly calibrated or adjusted when necessary, according to protocols for each instrument.

5.2. Validation

The techniques described above for the examination of physical fits are well known and scientifically accepted in the forensic science community and in private industry (e.g., fracture mechanics, engineering, and metallurgy). Relevant examples of related literature can be found in Section 6 (References).

5.3. Verifications

5.3.1. All probative physical fits (e.g., those that provide an association between a suspect and a scene or a suspect and a victim such as a roll of tape from a suspect's residence physically fits to a piece of tape on a pipe bomb) shall be verified by another qualified examiner (seconded).



ATF-LS-TE10 Examination of Physical Fits	ID: 1928 Revision: 6
Authority: Technical Leader	Page: 3 of 3
Original maintained by Quality Programs; copies are uncontrolled.	

5.3.2. Verifications shall be documented in the technical record in accordance with ATF-LS-7.7 Section 2.6 Casework Verification. The Physical Fit Verification Form can be used for such documentation.

6. References

Agron N, Schechter B. Physical Comparisons and Some Characteristics of Electrical Tape, AFTE J. 18 (1986) 53–59.

<https://doi.org/10.2174/0929866525666171214111007>

Bradley MJ, Keagy RL, Lowe PC, Rickenbach MP, Wright DM, LeBeau MA. A validation study for duct tape end matches, J. Forensic Sci. 51 (2006) 504–508.

<https://doi.org/10.1111/j.1556-4029.2006.00106.x>

Brooks E, Prusinowski M, Gross S, Trejos T. Forensic Physical Fits in Trace Evidence Discipline: A Review. Accepted for publication in Forensic Sci Int, May 2020.

De Forest PR, Gaensslen RE, Lee HC. Forensic Science: An Introduction to Criminalistics, McGraw-Hill, Inc., New York, NY, 1983.

Dixon KC. Positive Identification of Torn Burned Matches with Emphasis on Crosscut and Torn Fiber Comparisons, J. Forensic Sci. 28 (1983) 351–359.

Katterwe HW. Fracture Matching and Repetitive Experiments: A Contribution of Validation, AFTE J. 37 (2005) 229–241.

Kirk PL. Crime Investigation, 2nd Edition. Chapters 9, 17, 20. John Wiley and Sons: New York, NY 1974.

Thornton JI. Fractal Surfaces as Models of Physical Matches, J. Forensic Sci. 31 (1986) 1435–1438.

SWGDOC Standard for Physical Match of Paper Cuts, Tears, and Performations in Document Examinations. Ver. 2013-1.

Tsach T, Wiesner S, Shor Y. Empirical proof of physical match: Systematic research with tensile machine, Forensic Sci. Int. 166 (2007) 77–83.

<https://doi.org/10.1016/j.forsciint.2006.04.002>



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 1 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

1.1. The forensic fiber examiner can be requested to conduct a variety of examinations on textiles for the purposes of identifying and comparing types of fabric, cordage, damage. In addition, they may be requested to evaluate and compare fabric impressions.

1.2. Fiber Examinations

1.2.1. Usually, the forensic fiber examiner is requested to compare questioned and known (Q and K) samples based on their physical and chemical compositions. In conducting those comparisons, the forensic fiber examiner's goal is to assess the significance of any differences observed. The absence of any exclusionary differences between the Q and K samples suggests that the items could have had a common source of origin. Besides a Q vs. K comparison, the examiner may also be requested to analyze a questioned fiber and attempt to determine the possible source(s) of origin for that sample.

1.2.2. The physical, optical, and chemical properties of known and questioned fibers that may be part of an examination may include: Physical – color, cross-section, diameter, delusterant, surface characteristics; Optical – Polarized light microscopy (PLM) - birefringence, refractive index (indices), sign of elongation, and extinction characteristics; Chemical – micro-solubility/micro-chemical tests, Fourier transform infrared spectroscopy (FTIR), microspectrophotometry (MSP), and Pyrolysis Gas Chromatography-Mass Spectrometry (PyGC-MS).

1.2.2.1. The order of these examinations and any additional testing is left to the discretion of the examiner and based upon the evidence at hand. In bombing cases, fiber recovery from the device in question is of paramount importance. Generally, environmental (scene) fibers will be encountered in all such cases and have little to no probative value in the case. Fibers recovered from protected (pristine) areas of the device (i.e., under or in between multilayered tape) may be significant since their deposition could have been affected at the time the device was manufactured.

1.3. Fabric Damage

1.3.1. Textile items are occasionally submitted to the laboratory for examination to determine if the item has been damaged. The construction and composition of the textile are vital factors in assessing and understanding damage characteristics. Information as to the possible implement causing the damage and the manner in which it was caused may also be determined. Information from these examinations



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 2 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

may corroborate a crime scene scenario, refute particulars in a crime scene scenario, and/or assist with determination of death in decomposed bodies.

1.4. Fabric Impressions

1.4.1. Fabric impressions occur from the transfer of a fabric's construction pattern (i.e., weave, twill, stitching, seams) to the surface of another object. Impressions can be produced when the fabric leaves behind some material (i.e., blood, grease dirt) on the receiving object, or when a fabric removes a material from the receiving object. A three-dimensional impression is produced when a fabric is pressed into the receiving object to the extent that it embeds into the material (e.g., impression in mud). The process of analyzing impressions is a step-by-step methodical approach that uses class and randomly acquired characteristics found in known and unknown impressions.

2. Instrumentation/Reagents

2.1. Sticky-sided collecting materials such as tape or Post-it Notes

2.2. Forceps

2.3. Containers such as glassine envelopes, plastic bags, or vials

2.4. Illuminated magnifier

2.5. UV Light or alternative light source

2.6. Transparent securing substrates such as sheet protectors

2.7. Glass microscope slides

2.8. Glass coverslips

2.9. Mounting medium

2.10. Solvents/stains/microchemical reagents

2.11. Stereomicroscope, PLM, or comparison microscope

2.12. Microscope with fluorescence attachments



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 3 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

2.13. FTIR

2.14. MSP

2.15. PyGC-MS

2.16. High temperature silicone oil

2.17. Hot-Stage apparatus

2.18. Digital camera

3. Safety Considerations

3.1. The examiner should follow all biohazard procedures and use universal safety precautions.

3.2. Precautions need to be taken whenever working with chemicals which could pose potential health hazards.

4. Procedure or Analysis

4.1. Recovery of Fibers

4.1.1. Purpose

4.1.1.1. Items of evidence are examined for foreign fibers that may be associated with a known source. Document the condition of the submitted items (i.e., intact, buttons missing, apparent rips or tears) and include a brief description of any design, logos, or lettering present on evidence. Descriptions may include garment or textile label information such as fiber content, brand or manufacturer, manufacturer's numbers (e.g., RN# or WPL#), and the size.

4.1.2. Summary

4.1.2.1. Generally speaking, submitting the article(s) of evidence to the laboratory for the examiner to process is the best approach to the recovery of fibers. There are instances where this is not practical or possible, such as recovering fibers from wall-to-wall carpeting, a large piece of furniture,



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 4 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

or a vehicle. In these instances, the recovery may be accomplished at the scene with the aid of an alternative light source, if available, and the recovered fibers submitted for examination.

4.1.2.2. The recovery of fibers can be obtained by particle picking (manual removal) as well as tape lifting methods. Gentle scraping may be necessary in certain instances. Vacuuming can also be used to collect debris; however, it is not preferred because the debris recovered often represents far more than recent fiber transfers. The choice of recovery method is sample driven.

4.1.2.3. Multi-layered tape recovered directly from devices should be separated layer-by-layer and examined for any fibers or other evidence that could have originated from the environment in which the explosive device was manufactured. Latent print and DNA examinations may be performed before and/or after the tape is separated; therefore, the examiner shall handle the recovered tape with this in mind. Fibers of interest found in the pristine area of the tape are removed with clean forceps.

4.1.3. Minimum Standards and Controls for Recovery of Fibers

4.1.3.1. If possible, the victim's evidence and suspect's evidence should be examined in separate rooms. If this is not possible, then the separation of victim and suspect evidence in time and/or space will be necessary.

4.1.3.2. Clean the examination area and change the examination paper between processing victim and suspect or scene exhibits at a minimum.

4.1.3.3. Change gloves and clean tools between examining the evidence from the victim and the evidence from the suspect. Use separate laboratory coats during the collection of the known and questioned items.

4.1.3.4. Follow applicable biohazard procedures and use universal safety precautions.

4.1.4. Sample Selection

4.1.4.1. Many items such as tapes or garments will have too many fibers present on them to collect every fiber. Care should be taken to select a representative sample of each visually different fiber type for further analysis.



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 5 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

4.1.5. Analytical Procedure for Recovery of Fibers

- 4.1.5.1. Clean the examination area. Spread a clean piece of butcher or Kraft paper out on the examination surface.
- 4.1.5.2. Examine each item of evidence visually or with the aid of an illuminated magnifier, UV light, or other alternative light source(s).
- 4.1.5.3. If the item being examined contains fibers that are readily visible, collect them. As fibers are collected, they should be secured and/or preserved in an appropriate manner.
- 4.1.5.4. Care should be taken to avoid the loss of any fibers, especially when repositioning bulky items.
- 4.1.5.5. Adhesive tapes and/or other adhesive devices (e.g., “Post-it Notes”, lint rollers) may be used to recover fibers. The adhesive surface is placed on the item being examined and then pulled away.
- 4.1.5.6. Other collection methods may be used including vacuuming and scraping. If scraping is necessary, the item to be examined is suspended above the examination surface and very gently scraped with a spatula. Scraping in a downward direction allows surface fibers to fall onto the examination surface for collection. If vacuuming is necessary, then separate filters should be used for each item/area.
- 4.1.5.7. When recovering fibers from tape present on submitted items, fibers should be considered valuable evidence only if they are recovered from protected surfaces such as between layers of tape or between the tape and the item that the tape is adhering to. While some fibers of value may be found on exposed areas of the tape, the fact that environmental (scene) fibers having no probative value may also be present on these areas should be taken into consideration. Latent print and DNA considerations of these tape pieces are paramount as well as other trace evidence (see “Tape Protocol”). Multiple layers of tape should be separated layer-by-layer for examination. Remove any fibers from the freshly exposed adhesive area(s) and document. The exposed tape adhesive may be placed on a clean sheet of plastic, glass, or a screen for transfer to latent prints.

4.2. Fiber Identification



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 6 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

4.2.1. Purpose

4.2.1.1. When no known fibers/fabrics are submitted for comparison purposes, the unknown fibers may be characterized and identified as to their generic class/sub-class to identify a possible source of the fibers which may provide investigative leads. In these instances, fibers may be identified through stereomicroscopy and PLM only (although other instrumental methods may be used at the discretion of the analyst). Other analytical methods are employed when comparisons are to be conducted between known and unknown fibers.

4.2.2. Minimum Standards and Controls for Fiber Identification

4.2.2.1. A reference collection of fibers may be useful to the examiner when identifying the generic class and/or sub-generic classes.

4.2.2.2. Reference information such as a collection of FTIR spectra and tables of physical and optical properties of known fibers are desirable.

4.2.3. Sample Selection

4.2.3.1. Fibers should first be examined using a stereomicroscope. The different physical characteristics should be observed. Fibers may be mounted on glass slides as deemed necessary. When numerous fibers are present in a questioned sample, the examiner will evaluate the fibers on a case-by-case basis and should attempt to mount a representative sample of fibers that display the range of variation seen within the sample.

4.2.3.2. If several questioned fibers are recovered which are to be identified, they shall be characterized using the PLM. If it is concluded that all the questioned fibers are consistent in fiber type, color, diameter, cross-sectional shape, and optical properties to one another, additional analysis (e.g., FTIR, MSP) can then be performed on a select few of the questioned fibers. The report shall clearly state that the results are based only on the portion(s) tested.

4.2.4. Analytical Procedure for Fiber Identification

4.2.4.1. Observe and record the physical and optical properties of the fibers utilizing the PLM. Classify the fiber type based on the characteristics noted if necessary.



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 7 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

- 4.2.4.2. When necessary, obtain FTIR spectra of the fiber and compare the spectrum obtained with reference spectra of fibers.
- 4.2.4.3. Solubility/staining/micro-chemical tests may be conducted.
- 4.2.4.4. If desired, a cross-section of the fiber may be made using appropriate techniques.
- 4.2.4.5. Other analytical techniques commonly used for the comparison of fibers may be used as deemed necessary.

4.3. Comparison of Fibers

4.3.1. Purpose

- 4.3.1.1. In some cases, a submitted known sample of fibers/fabric is characterized, identified, and used for comparison to questioned fibers recovered on probative items to determine if they could have originated from the same source. In addition, questioned fibers can be compared from different scenes/locations.

4.3.2. Minimum Standards and Controls for Comparison of Fibers

- 4.3.2.1. Use a comparison microscope and/or the PLM when comparing known and questioned fibers.
- 4.3.2.2. Use a suitable known fiber sample to obtain the best and most reliable results in a fiber comparison.

4.3.3. Sample Selection

- 4.3.3.1. **Known Fibers:** When a known sample of fibers/fabric is submitted, the scientist can treat the sample as a single source even if different fiber types/colors are present. Knowledge of the manufacturing process for the types of fiber evidence encountered in casework as well as a visual examination of the fibers present in the sample, aids in choosing an appropriate representative known sample. A known sample should consist of enough fibers to represent the different fiber types/colors present in the sample.
- 4.3.3.2. **Questioned Fibers:** If several questioned fibers are recovered for comparison, they shall be characterized and compared using the PLM. If



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 8 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

it is concluded that a group of the questioned fibers are consistent in fiber type, color, diameter, cross-sectional shape, and optical properties with one another, additional analysis (e.g., FTIR, MSP) can be performed on a select few of those questioned fibers. The report should be clear that the results are based only on the portion(s) tested.

4.3.4. Analytical Procedures for the Comparison of Fibers

- 4.3.4.1. When comparing fibers, the same analytical techniques shall be performed in the same manner on both the known and questioned when possible.
- 4.3.4.2. At any time during the fiber examination scheme, if exclusionary differences are detected between the fibers, a conclusion can be made that the fibers do not have a common origin and no further examination/comparison is necessary.
- 4.3.4.3. Generally, when sample size is limited, destructive testing is performed after all non-destructive testing is complete.
- 4.3.4.4. Comparison microscopy, PLM, and/or fluorescence microscopy should be conducted with all fiber comparisons.
- 4.3.4.5. FTIR should be conducted when man-made (synthetic) fibers are to be compared (regenerated cellulosic fibers may be analyzed at the examiners discretion). Compare the spectra. Any exclusionary difference between the two is reason for elimination.
- 4.3.4.6 MSP should be considered when colored fibers are to be compared (although very light fibers or very dark fibers may not produce useful results). It may be necessary to obtain several spectra along the length of a given fiber or from several different fibers of the same color to determine the reproducibility of the spectra. Any exclusionary difference between the compared fibers is reason for elimination.
- 4.3.4.7 PyGC-MS may be conducted. . Any exclusionary difference in the resulting data between the compared fibers is reason for elimination.

4.4. Hot Stage Microscopy

4.4.1. Purpose



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 9 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

4.4.1.1. There may be instances where observing the melting point behavior of thermoplastic fibers under the microscope may provide valuable information for fiber identification, sub-classification, and/or comparison.

4.4.2. Minimum Standards and Controls for Hot Stage Microscopy

4.4.2.1. The hot stage apparatus shall be capable of reaching at least 300°C and should fit the stage of the PLM. A clear image of the fiber should be visible by transmitted light at a magnification of at least 100X. The temperature of the hot stage should be able to be raised by as little as 4°C per minute or less. The hot stage should be performance checked and adjusted with melting point standards within 30 days of running the casework samples if using for fiber identification or sub-classification.

4.4.3. Analytical Procedures for Hot Stage Microscopy

4.4.3.1. Fibers may be mounted in air or in high temperature silicon oil. Only a small length of fiber is necessary.

4.4.3.2. The melting point range observations are made through the PLM. The melting point range (when the fiber starts to melt and has completely melted) should be recorded.

4.4.3.3. Multiple measurements should be considered when determining fiber identification, sub-classification, and/or comparison. The number of measurements taken is left to the discretion of the examiner and may be based on sample size.

4.4.3.4. Thermal microscopy is a destructive technique. All non-destructive techniques should be performed before destructive techniques.

4.5. Natural Fibers

4.5.1. Purpose

4.5.1.1. Distinguish between the different types of natural fibers used in fabric and cordage.

4.5.2. Minimum Standards and Controls for Natural Fiber Examinations

4.5.2.1. A reference collection is useful when examining natural fibers. When chemicals or stains are used, examine a reference fiber side-by-side with



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 10 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

the questioned and known fibers and subject each to the same conditions and stains to assure the chemicals/stains are working properly.

4.5.3. Analytical Procedures for Natural Fiber Examinations

- 4.5.3.1. Fibers should be first examined using a stereomicroscope. The different physical characteristics should be noted.
- 4.5.3.2. Observe the physical and optical properties of the fibers utilizing the PLM. Note the extinction properties of the fibers (e.g., full, incomplete, undulating, or no extinction). Regarding plant fibers, it may be necessary to separate the bundles of fibers into ultimates. There are many different procedures for macerating the bundles. Note any microscopical observations (e.g., size and shape of the lumen, presence of nodes, presence of spirals, presence of scales)
- 4.5.3.3. The Herzog Test may be used to classify/identify the various types of natural fibers. Examine the fibers using a full wave plate (analyzer engaged) to determine the twist of the fiber and note whether the reaction is weak or strong.
- 4.5.3.4. Dispersion staining and dry twist tests may also be useful in distinguishing between the various types of natural fibers. A number of stains (e.g., Graff's C Stain, Herzberg Stain) are available and may be used to further distinguish the natural fibers.

4.6. Fabric Damage

4.6.1. Purpose

- 4.6.1.1. Textile items can be submitted to the laboratory for examination to determine if the item has been damaged. The construction and composition of the textile are important factors in assessing and understanding damage characteristics. Information as to the possible cause (i.e., tool, device, heat) of the damage may also be determined.

4.6.2. Analytical Procedure for Fabric Damage Examinations

- 4.6.2.1. The procedures for textile damage determination depend on case specifics as well as the evidence received/examined. In general, the steps to be taken are as follows:



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 11 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

- 4.6.2.1.1. Textile damage examinations can be complex and should be approached in context with case specific information. Therefore, the examiner should attempt to gain all the information that may account for the presence of any noted damage (e.g., scissor cuts created by first responders).
- 4.6.2.1.2. Conduct a visual examination of the textile. Suspected damage should be approached from the largest to the smallest scale (i.e., fabric, yarn, and fiber).
- 4.6.2.1.3. Examine and document the damage in detail. Some characteristics that may be visible and documented include FABRIC: length, distortion, curl, shape, secondary cuts, steps, coloration; YARN: unraveling, isolated threads, planar array, ragged ends, steps, ruptured ends; FIBERS: splayed out, clean-cut ends, bulbous formation, melting.
- 4.6.2.1.4. Perform simulation experiments if necessary. This should be done on an undamaged area of the submitted item if possible. Clearly mark any damage produced by the examiner.
- 4.6.2.1.5. Evaluate the visible characteristics of the damage, considering the limitations, and make a conclusion.

4.7. Fabric Impressions

4.7.1. Purpose

- 4.7.1.1. Fabric impression evidence is produced when an object or material retains the characteristics of a textile material that has been pressed against it. The process of analyzing impressions is a step-by-step methodical approach that uses class and randomly acquired characteristics found in known and unknown impressions.

4.7.2. Analytical Procedure for Fabric Impression Examinations

- 4.7.2.1. All examinations, relevant observations, and results shall be documented in the examination records and support conclusions reached. Examinations may be terminated once an exclusionary difference is established.
- 4.7.2.2. Detection/Collection/Processing



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 12 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

4.7.2.2.1. Impressions can be submitted to the laboratory in various forms (e.g., digital images, impressions on objects, lifts, casts). These impressions will be located using oblique light, alternative light source, and/or digital, chemical, or physical enhancement. They may be captured using photography, scanning, lifting, and/or casting. They may also be processed digitally, physically, and/or chemically, to prepare for examination and/or optimize visibility. See also *ATF-LS-11*.

4.7.2.3. Suitability

4.7.2.3.1. The unknown impression needs to be assessed to determine whether it is suitable for comparison. Unsuitable impressions lack sufficient detail and will prevent meaningful comparisons with a known source. The quantity (how much of the impression is present) and quality (clarity) of detail are assessed. This assessment is dependent on several factors such as the substrate, interferences, and the presence or absence of scales. These factors may limit or qualify an examiner's conclusions.

4.7.2.4. Known impressions

4.7.2.4.1. To compare a questioned impression to a known fabric, clear and concise prints should be made with the known. The purpose of creating known test impressions is to record the characteristics on the fabric. Prior to making known impressions, the examiner should recognize and preserve other relevant physical evidence as well as document and photograph the original condition of the fabric. The case specifics will determine the number and types of impressions to be made.

4.7.2.5. Class characteristic comparison

4.7.2.5.1. This comparison can be a side-by-side comparison and/or a superimposed observation of the unknown impression with the known fabric impression.

4.7.2.5.2. Class characteristics such as specific design, weave, spacing, manufacturing characteristics and shape of the design, are evaluated and compared.



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 13 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

4.7.2.6. Randomly acquired characteristic comparison

- 4.7.2.6.1. This comparison can be a side-by-side comparison and/or a superimposed observation of the unknown impression with a known fabric impression.
- 4.7.2.6.2. Randomly acquired characteristics are evaluated according to their position, size, shape, orientation, and clarity.
- 4.7.2.6.3. Randomly acquired characteristics present in both the unknown impression and the known impression shall be confirmed on the fabric itself when possible.
- 4.7.2.6.4. When sufficient randomly acquired characteristics are present in the unknown impression and correspond with features on the known object, a positive identification can be made.
- 4.7.2.6.5. Positive identifications shall be evaluated by a second qualified examiner (verifier). The verification must be conducted to the extent that the verifier could independently defend and testify to the same conclusions. Verification shall be documented in the technical record by the verifiers signature.

5. Quality Assurance and Controls

- 5.1. Through proper training, competency testing, and proficiency testing of fiber examiners as well as the use of high-quality microscopes and equipment which are appropriately cleaned, maintained, and quality checked (e.g., calibrated, performance checked), the quality of this method is assured.
- 5.2. Because fibers are mass produced, a questioned fiber can never be positively identified back to a specific source; therefore, the use of error rates is not applicable.

5.3. Validation

- 5.3.1. The techniques described above for textile examinations are well known and scientifically accepted in the forensic science community and private industry. Relevant examples of related literature can be found in Section 6 (References).

6. References

6.1. ANSI/ASB Standards



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 14 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

Best Practice Recommendation 021, Best Practices for the Preparation of Test Impressions from Footwear and Tires

Best Practice Recommendation 049, Best Practices for Lifting of Footwear and Tire Impressions

6.2. ASTM International Standards

ASTM E1459 Standard Guide for Physical Evidence Labeling and Related Documentation

ASTM E1492 Standard Practice for Receiving, Documenting, Storing and retrieving Evidence in a Forensic Science Laboratory

ASTM E2224 Standard Guide for Forensic Analysis of Fibers by Infrared Spectroscopy

ASTM E2225 Standard Guide for Forensic Examination of Fabrics and Cordage

ASTM E2228 Standard Guide for Microscopic Examination of Textile Fibers

6.3. Scientific Working Group for Materials Analysis (SWGMAT) Documents found at <http://www.asteetrace.org>

Forensic Fiber Examination Guidelines

- *“Introduction to Fibers Chapter” (2011 Update)*
- *“Microscopy Chapter” (2011 Update)*
- *“UV-VIS Spectroscopy of Textile Fibers Chapter” (2011 Update)*

6.4. Others

Gaudette, B.D. In Forensic Science Handbook; Saferstein, R., Ed.; Prentice Hall: Englewood Cliffs, N.J., 1988; Vol. II, Chapter 5

Gross, S. Fabric Damage: “Cuts, tears, burns and others.” Presentation given at Advance Trace Evidence Symposium, June 2006, Ames, IA located on Burshare drive.



ATF-LS-TE11-Examination, Analysis, and Comparison of Textiles	ID: 1929 Revision: 5
Authority: Technical Leader	Page: 15 of 15
Original maintained by Quality Programs; copies are uncontrolled.	

Nielsen, Mark, R., "Common Natural Fibers". Handout provided at a paper presentation at the Midwestern Association of Forensic Scientists annual meeting, October 1998

Palenik, Samuel, J., Microscopical Examination of Fibres. In: Forensic Examination of Fibres. 2nd ed., James Robertson and Michael Grieve, Philadelphia, 1999.

Petraco, N. and Kubic, T. Color Atlas and Manual of Microscopy for Criminalists, Chemists, and Conservators. CRC Press, Boca Raton, 2004.

Robertson J, Grieve M. Forensic Examination of Fibres 2nd Edition, Taylor & Francis, 1999.

Schubert, Glenn, "Fabric Impression Workshop" PowerPoint presentation from IPES located on Burshare drive.



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 1 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

- 1.1. When tape is received as evidence, a multi-disciplinary approach must be considered. Latent print examiners, trace evidence analysts, and scientists from any other discipline involved should work together to devise a scheme of analysis so as to glean as much information as possible for all disciplines. The initial examiner may examine the tape for trace evidence, or the tape could be transferred to a trace evidence examiner for examination and recovery of any trace evidence on the tape. Prior to latent print processing, a sample of tape may be removed or preserved for possible future tape examinations. An attempt should be made to take the sample from a portion of the tape which will be least likely to contain fingerprints. Care should be taken when processing the ends of the tape to minimize damage to the torn ends, preserving the ends for a possible physical fit. If tape needs to be cut from an item, any cuts made by an examiner should be made and/or labeled in such a way as to be easily recognized (e.g., zigzag cut, exaggerated angle cut).
- 1.2. Quite frequently, glue/adhesive/sealant/filler material (hereafter simply referred to as “adhesive”) will not be inventoried as a separate item but will be a component of the exhibit being examined (e.g., part of the tape, device component). Adhesives should be examined for the inclusion of trace evidence on or embedded in the adhesive.
- 1.3. Reference(s) to applicable OSAC Registry documents
 - 1.3.1. ASTM E3085 Standard Guide for Fourier Transform Infrared Spectroscopy in Forensic Tape Examinations
 - 1.3.2. ASTM E3260 Standard Guide for Forensic Examination and Comparison of Pressure Sensitive Tapes
 - 1.3.3. ASTM E3233 Standard Practice for Forensic Tape Analysis Training Program

2. Instrumentation/Reagents

- 2.1. Tweezers, scalpel, and other appropriate tools
- 2.2. UV light
- 2.3. Appropriate solvents (chloroform, toluene, etc.)
- 2.4. Micrometer and other measuring devices
- 2.5. Microscopes
 - 2.5.1. Polarized light microscope



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 2 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

2.5.2. Stereomicroscope

2.6. Glass microscope slides and coverslips

2.7. Mounting media

2.8. Camera or other Imaging Equipment

2.9. Instrumentation

2.9.1. FTIR (*ATF-LS-E6*)

2.9.2. MSP (*ATF-LS-TE03*)

2.9.3. Pyrolysis GC-MS or High Temperature GC-MS (*ATF-LS-TE04, ATF-LS-FD2*)

2.9.4. XRD (*ATF-LS-E5*)

2.9.5. XRF or SEM-EDS (*ATF-LS-E4, ATF-LS-E3*)

3. Safety Considerations

3.1. The examiner shall follow all the biohazard procedures and use universal safety precautions.

3.2. Precautions need to be taken whenever working with chemicals which could pose potential health hazards.

4. Procedure or Analysis

4.1. Minimum standards and controls

4.1.1. The examiner shall clean the examination area and/or change the examination paper between questioned and known samples and when it seems appropriate.

4.1.2. The examiner shall clean their tools between samples.

4.1.3. If at any time during the comparative scheme of analysis an exclusionary difference is observed between the Q and the K samples, no further examinations



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 3 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

need to be conducted and the tapes or adhesives can be reported as being dissimilar to one another.

4.2. Physical Fit for tapes and adhesives

4.2.1. If a physical fit is made, no further chemical analysis is required. Refer to Examination of Physical Fits protocol (*ATF LS TE10*).

4.3. Sample selection/Representative sample

4.3.1. Sample selection

4.3.1.1. Each recovered piece of questioned tape or adhesive should be examined unless the number of pieces makes this procedure prohibitive. In that case, select sample(s) may be taken for further analysis. Because different/separate tape or adhesive pieces cannot be assumed to be from the same source, sample selection shall be utilized when reporting the examination of questioned samples.

4.3.2. Representative sample

4.3.2.1. Questioned sample: When testing individual questioned pieces of tape or clumps of adhesive, certain tests may be conducted on smaller samples which are removed from that larger piece or clump. In that instance, homogeneity is assumed. Accordingly, the results of those tests may be used to represent the larger piece (or pieces that have been physically fit together) as a whole.

4.3.2.2. Known sample: It can be assumed that the known tape from a roll or known adhesive from a tube is homogeneous and therefore a representative sample from the known can be utilized and reported.

4.4. Chemical Analysis for tapes and adhesives

4.4.1. Purpose

4.4.1.1. Chemical analyses are performed on tapes and adhesives to aid in the identification of the source and/or for comparison between tapes and adhesives.

4.4.2. Analytical Procedure - Tape



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 4 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

The analytical scheme will vary depending on the type of tape and if it is a characterization or a comparison.

4.4.2.1. Characterization: The minimum analysis for the characterization of tape includes:

Visual and/or microscopic examination to determine type of tape (e.g., duct, electrical).

If any chemical information is reported, instrumental analysis is required (e.g., reporting polyvinyl chloride).

4.4.2.2. Comparison: The minimum analytical scheme for comparison of tapes includes physical characterization and separate analysis of each major component (backing, adhesive, and reinforcing material, if present). This analysis must include the use of at least two instrumental techniques (one for organic and one for elemental analysis) for the backings and adhesives. The questioned item is evaluated to identify physical characteristics (e.g., color, layer structure, dimensions) suitable for comparison prior to examination of the known tape. Any subsequent chemical and elemental analysis of the unknown item shall be conducted prior to the known item.

Duct tape (i.e., poly-coated cloth tape)

- Physical characteristics that may be evaluated include:
 - § Color (backing and adhesive)
 - § Width
 - § Thickness
 - § Backing texture
 - § Scrim count (yarns per square inch)
 - § Adhesive by UV light
 - § Cross section of backing and adhesive
 - § PLM of adhesive
- Analysis of reinforcing material including construction and composition. Examine the fibers per protocol for the Examination, Analysis and Comparison of Textiles (*ATF LS TE11*)
- Instrumental analysis techniques for backing and adhesive:
 - § FTIR
 - § Raman
 - § PGCMS



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 5 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

- § SEM-EDS
- § XRF
- § XRD
- § MSP (backing only)

Electrical tape (i.e., vinyl tape)

- Physical characteristics that may be evaluated include:
 - § Color of backing and adhesive
 - § Width
 - § Thickness
 - § Backing texture
 - § Cross section of backing and adhesive
 - § PLM of adhesive

- Instrumental analysis techniques for backing and adhesive:
 - § FTIR
 - § Raman
 - § PGCMS
 - § SEM-EDS
 - § XRF
 - § MSP (backing)

Other tapes (i.e., packaging tape, masking tape, filament tape, office tape)

- Physical characteristics as previously described
- Chemical analysis of backing and adhesive as previously described
- Fibers or fabric analysis including construction and composition.
 - Examine the fibers per protocol for the Examination, Analysis and Comparison of Textiles (*ATF LS TE11*)
- Clear packaging tapes should be examined by PLM and the following can be determined and/or compared:
 - § Extinction angle relative to the machine edge
 - § Retardation colors of the tapes
 - § Monoaxially oriented polypropylene (MOPP) or biaxial oriented polypropylene (BOPP) films
 - § If the films are BOPP, determine the BOPP angles



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 6 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

4.4.3. Analytical Procedure – Adhesives

The analytical scheme will vary depending on the type of adhesive and if it is a characterization or a comparison.

4.4.3.1. Characterization: The minimum analysis for the characterization of an adhesive includes:

Visual and/or microscopic examination to report that an adhesive is present.

If any chemical information is reported, instrumental analysis is required (e.g., reporting styrene butadiene, silicone, epoxy)

4.4.3.2. Comparison: The minimum analysis for the comparison of adhesives includes physical characterization and instrumental analysis to include the use of at least two instrumental techniques (one for organic and one for elemental analysis). The questioned item is evaluated to identify physical characteristics (e.g., color, opacity, texture) suitable for comparison prior to examination of the known adhesive. Any subsequent chemical and elemental analysis of the unknown item shall be conducted prior to the known item.

If dried adhesives are to be compared with liquid materials from a tube or bottle, a known comparison standard sample shall be prepared by mixing the sample, if necessary, applying a portion of the sample to a clean glass slide and allowing the sample to thoroughly dry/cure. In some instances (such as with moisture cure adhesives) the adhesive may need to be placed in a moist environment and may need to be heated to facilitate complete curing. Ensure that the sample is protected from any dust or contamination while it is being cured.

Physical characteristics that may be evaluated include:

- § Color
- § Texture
- § Solubility
- § Elasticity
- § Porosity
- § Opacity
- § UV
- § PLM



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 7 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

Instrumental analysis techniques:

- § FTIR
- § Raman
- § PGCMS
- § SEM-EDS
- § XRF
- § XRD

5. Quality Assurance and Controls

- 5.1. Through proper training and competency testing of examiners, and through the use of high-quality equipment, which is appropriately cleaned, maintained and quality checked (e.g., calibrated, performance checked), the quality of this method is assured.
- 5.2. Because tapes and adhesives are mass produced, a questioned tape or adhesive can never be positively identified back to a specific source unless a physical fit is confirmed.
- 5.3. Follow each instrument protocol regarding performance checks and the use of appropriate standards, controls and blanks.

5.4. Validation

- 5.4.1. The techniques described above for tapes and adhesive examination are well known and scientifically accepted in the forensic community and in private industry. Relevant examples of related literature can be found in Section 6 (References).

6. References

6.1. ASTM International Standards

E2809 Standard Guide for Using Scanning Electron Microscopy/X-ray Spectrometry in Forensic Polymer Examinations

E3296 Standard Guide for Using Pyrolysis Gas Chromatography and Pyrolysis Gas Chromatography-Mass Spectrometry in Forensic Polymer Examinations

- 6.2. Scientific Working Group for Materials (SWGMAAT) Documents available at: www.asteetrace.org



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 8 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

SWGMAAT Guideline for Assessing Physical Characteristics in Forensic Tape Examination

SWGMAAT Guideline for Using Light Microscopy in Forensic Tape Examinations

6.3. Other

Agron N, Schechter B. Physical comparisons and some characteristics of electrical tape. AFTE Journal, Vol. 18, No. 31, 1986, pp. 53-591.

Bakowski NL, Bender EC, Munson TO. Comparison and identification of adhesives used in improvised explosive devices by pyrolysis-capillary column gas chromatography-mass spectrometry. Journal of Analytical and Applied Pyrolysis, Vol. 8, 1985, pp.483-492.

*Benson JD. Forensic examination of duct tape. Proceedings of the International Symposium on the Analysis and Identification of Polymers, 1984, pp.145-146. FBI Academy, Quantico, VA. Retrieved from:
https://drive.google.com/file/d/0B1RLIs_mYm7edI92c0hDNklGTTg/view*

Bradley MJ, Gauntt JM, Mehlretter AH, Lowe PC, Wright DM. A Validation Study for Vinyl Electrical Tape End Matches. Journal of Forensic Sciences. 2011;56(3):606–611.

Bradley MJ, Keagy RL, Lowe PC, Rickenbach MP, Wright DM, LeBeau MA. A validation study for duct tape end matches. Journal of Forensic Sciences. 2006;51(3):504–508.

Flick EW. Adhesive and Sealant Compound Formulations, Park Ridge, NJ: Noyes Publications 1984.

Forensic Science Handbook, Volume III, Richard Saferstein, ed.; Regents/ Prentice Hall 1993 (especially chapter 4 for infrared analysis)

Goodpaster JV, Sturdevant AB, Andrews KL, Briley EM, Brun-Conti L. Identification and comparison of electrical tapes using instrumental and statistical techniques: II Organic composition of the tape backing and adhesive. Journal of Forensic Sciences, Vol. 54, No. 2, 2009, pp. 328-338.



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 9 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

Goodpaster JV, Sturdevant AB, Andrews KL, Brun-Conti L. Identification and comparison of electrical tapes using instrumental and statistical techniques: I Microscopic surface texture and elemental composition. Journal of Forensic Sciences, Vol. 52, No. 3, 2007, pp. 610-629.

Gross S, Jorstad J. Analysis and discrimination of colored pressure sensitive tape backings by , offimicrospectrophotometry (MSP). Journal of American Society of Trace Evidence Examiners, Vol. 9, No. 1, pp. 17-36.

Jenkins Jr TL. Elemental examination of silver duct tape using energy dispersive x-ray spectrometry. Proceedings of the International Symposium on the Analysis and Identification of Polymers, 1984, pp. 147-149. FBI Academy, Quantico, VA.

Retrieved from:

https://drive.google.com/file/d/0B1RLIs_mYm7eTUDXVlo5WVFGRRHM/view

Johnston J. Pressure Sensitive Adhesive Tapes, Pressure Sensitive Tape Council, 2003.

Kee TG. The characterization of PVC adhesive tape. Proceedings of the International Symposium on the Analysis and Identification of Polymers, 1984, pp. 77-85. FBI Academy, Quantico, VA. Retrieved from:

https://drive.google.com/file/d/0B1RLIs_mYm7eWU9sdGFuMk1EVRG8/view

Keto RO. Forensic characterization of black polyvinyl chloride electrical tape. Proceedings of the International Symposium on the Analysis and Identification of Polymers, 1984, pp. 137-143. FBI Academy, Quantico, VA. Retrieved from:

https://drive.google.com/file/d/0B1RLIs_mYm7eZFZfWHNmTUNEUUK/view

Mehltretter AH, Bradley MJ. Forensic analysis and discrimination of duct tapes. Journal of the American Society of Trace Evidence Examiners, Vol. 3, No. 1, 2012, pp. 2-20.

Mehltretter AH, Bradley MJ. Forensic analysis and discrimination of duct tapes. Journal of the American Society of Trace Evidence Examiners, Vol. 3, No. 1, 2012, pp. 2-20.

Mehltretter AH, Bradley MJ, Wright DM. Analysis and discrimination of electrical tapes: Part I Adhesives. Journal of Forensic Sciences, Vol. 56, No. 1, 2011, pp. 82-94.



ATF-LS-TE13-Examination, Analysis, and Comparison of Pressure Sensitive Tapes (PST) and Adhesives	ID: 1931 Revision: 6
Authority: Technical Leader	Page: 10 of 10
Original maintained by Quality Programs; copies are uncontrolled.	

Mehltretter AH, Bradley MJ, Wright DM. *Analysis and discrimination of electrical tapes: Part II. Backings. Journal of Forensic Sciences, Vol 56 No. 6, 2011 pp. 1493–1504.*

Mehltretter AH, Wright DM, Dettman JR, Smith MA. *Intra-roll and intra-jumbo roll variation of duct tapes. Journal of the American Society of Trace Evidence Examiners, Vol. 6, No. 1, 2015, pp. 21-41.*

Mehltretter AH, Wright DM, Smith MA. *Variation in duct tape products over time: Physical measurements and adhesive compositional analysis by Fourier transform infrared spectroscopy. Forensic Chemistry, Vol. 4, 2017, pp. 1-8.*

Merrill RA, Bartick EG. *Analysis of pressure sensitive adhesive tape: I. Evaluation of infrared ATR accessory advances. Journal of Forensic Sciences, Vol. 45, No. 1, 2001, pp. 93-8.*

Microscopy and Microchemistry of Physical Evidence, Skip Palenik, in Forensic Science Handbook, Vol. II, ed. by Richard Saferstein, Prentice Hall 1988.

Patrick, RL. *Treatise on adhesion and adhesives. New York, NY: Marcel Dekker, Inc., 1967.*

Roth L. *Adhesives: General applications, theory, and testing. Appleton, WI: The Institute of Paper, 1968.*

Saferstein, Richard, "Criminalistics: An Introduction to Forensic Science" Prentice-Hall, In., 1995, pp. 65-67.

Smith J. *The forensic value of duct tape comparisons. Midwestern Association of Forensic Scientists Newsletter, Vol. 27, No. 1, 1998, pp. 28-33.*

Snodgrass H. *Duct tape analysis as trace evidence. Proceedings of the International Symposium on Trace Evidence, 1991, pp. 69-73. FBI Academy, Quantico, VA.*

Retrieved from:

https://drive.google.com/file/d/0B1RLIs_mYm7eQTNiZ3piUktnYlk/view

Williams ER, Munson TO. *The comparison of black polyvinyl chloride (PVC) tapes by pyrolysis gas chromatography. Journal of Forensic Sciences, Vol. 33, No. 5, 1988, pp. 1163-70.*



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 1 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

1.1. Any substance or item that may be taken away from a crime scene or left at a crime scene by the suspect or victim may become important evidence. For this reason, a veritable plethora of different types of substances may become evidence in a case. These types of materials may include but are in no way limited to items such as wood, paper, leather, feathers, matches, soils, tobacco, and household goods such as cleaning products or food items. As a part of the investigation, the trace evidence examiner may be asked on occasion to identify or compare these types of items. It is impossible to design a single analytical scheme which is capable of analyzing or identifying all substances. Due to this fact, the examiner must utilize common methods, laboratory equipment, and known reference materials or standards to affect identifications and/or conduct a comparison as needed on a case-by-case basis

2. Instrumentation/Reagents

2.1. Due to the wide variety of substances that may be encountered, the following is a list showing some of the equipment and/or materials which may commonly be used:

2.1.1. Stereomicroscope

2.1.2. Microscope with high magnification such as polarized light microscope or comparison microscope (*ATF-LS-TE02*)

2.1.3. Instruments

2.1.3.1. SEM-EDS (*ATF-LS-E3*)

2.1.3.2. XRF (*ATF-LS-E4*)

2.1.3.3. XRD (*ATF-LS-E5*)

2.1.3.4. GC-MS or Py-GCMS (*ATF-LS-E9 / ATF-LS-TE04*)

2.1.3.5. FTIR (*ATF-LS-E6*)

2.1.3.6. Microspectrophotometer (MSP) (*ATF-LS-TE03*)

2.1.4. Hot-stage Microscopy

2.1.5. Miscellaneous solvents and/or chemicals



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 2 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

2.1.6. Glass microscope slides, cover slips, mounting media

2.1.7. Litmus paper

3. Safety Considerations

3.1. Use appropriate safety garments and apparatus (i.e., glasses, gloves, lab coat)

3.2. Care shall be taken when handling chemicals and/or any physical evidence

4. Procedures

4.1. General Information

4.1.1. When attempting to identify general unknown substances, contact with the investigating officer prior to any analyses may provide useful information about items related to the victim, suspect, or crime scene. This could prove useful in narrowing down potential sources or possible identity of the general unknown in question. When a particular substance is suspected or known to the examiner as a possible source/identity of the unknown item of evidence, it may prove useful to call the manufacturer of the consumer product for information about product processing, ingredients, and packaging. Internet searches are also a good source of information.

4.2. Visual Examination

4.2.1. Visual examination of the submitted item is often the first step in identification or comparison of general unknowns or uncommon evidence items. Low power magnification may be used when applicable. This may be the only step necessary to affect an identification of some evidence items. Any significant physical characteristics such as size, color, texture, shape, or odor should be noted.

4.2.2. If the specimen is a liquid, check for sediments, suspensions, and any liquid interface. Foaming upon shaking may indicate soap or detergent. Items such as soap, detergents and cleaning powders are frequently encountered in criminal complaints

4.3. Procedure



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 3 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

4.3.1. Due to the wide range of samples encountered in this type of case work, the type of analyses conducted on the specimen will be determined on a case by case basis. Using the case history, the type of sample submitted as a guide if available, and the observations made during the visual examination; the examiner should decide which analytical methods are appropriate. The following are just a few of the common laboratory methods that may be utilized:

4.3.1.1. Microscopy

4.3.1.1.1. Microscopical examinations may lead to identification of the unknown substance and may be the only method necessary for comparison of some uncommon evidence items. General morphology as well as observation of the substance under controlled lighting conditions will aid in the identification and comparison. The nature and type of material will dictate what sample preparation is needed as well as what microscope(s) will be utilized. Starch, fungus, soil, feathers, leather, wood, paper, and plant material are just a few of the substances which can be identified and compared using stereomicroscopy and polarized light microscopy (See *TE02 Set-up and Use of the Microscope*).

4.3.1.2. pH

4.3.1.2.1. Test pH of a liquid sample and if possible compare to pH of control. If pH is unusual, the examiner may test for acids or bases—typical are hydrochloric acid and sodium hydroxide (See Appendix I).

4.3.1.3. Volatile and halogenated compounds

4.3.1.3.1. If unusual odors are present, consult with a fire debris chemist for the best way to proceed. Some halogenated compounds can be detected by spot tests (See Appendix I).

4.3.1.4. Toxic metals

4.3.1.4.1. Toxic metals can be detected by using the Reinsch test. This test can be applied directly to body fluids, tissue slurries, food and drink. Mercury, arsenic, silver, bismuth and antimony can be detected with this test (See Appendix I).

4.3.1.5. Organic substances



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 4 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

4.3.1.5.1. Water extractions are sometimes needed to test for inorganic substances. Silver nitrate and barium chloride are good reagents for general testing of samples for cyanide, arsenic and numerous anions. Silver nitrate, barium chloride and other reagents are described in Appendix I.

4.3.1.6. Acids/bases

4.3.1.6.1. Acidic/Basic organic extractions can be tested for the presence of drugs, pesticides and other organic substances on the GC-MS. The extraction may include clean up steps to eliminate unwanted compounds, e.g., fats.

4.3.1.7. Instrumentation

4.3.1.7.1. Some solid samples may be analyzed and compared on a variety of laboratory instruments such as the FTIR, SEM-EDS, XRF, XRD, MSP, or Py-GCMS (See individual instrument protocols listed above).

4.3.1.8. Specific analysis

4.3.1.8.1. Microchemical Tests (see Appendix I)

4.3.1.8.1.1. Chemical spot tests (color tests) can be used to indicate the presence of functional groups within the sample. Generally, the functional group is indicated to be present through the formation of a colored complex, a precipitate or the release of a gas. Microscopical crystal tests can be used on organic and inorganic compounds to characterize and possibly identify them by their crystal shape. Once a crystal has been characterized, its identity may be confirmed utilizing other instrumental techniques. The term microchemistry will be applied to both chemical spot tests and crystal tests.

4.3.1.8.2. Bank dyes and lachrymators (see Appendix II)

4.3.1.8.2.1. Chemical spot tests (color tests) can be used to indicate the presence of functional groups within the sample. Generally, the functional group is indicated to be present through the formation of a colored complex, a



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 5 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

precipitate or the release of a gas. Microscopical crystal tests can be used on organic and inorganic compounds to characterize and possibly identify them by their crystal shape. Once a crystal has been characterized, its identity may be confirmed utilizing other instrumental techniques. The term microchemistry will be applied to both chemical spot tests and crystal tests.

4.3.1.8.3. Building Materials (see Soil – Appendix IV and Wood – Appendix V)

4.3.1.8.3.1. Building materials vary with respect to physical and chemical features. The same general methods for soil can be applied to certain aspects of building materials such as plaster, concrete, sheetrock and masonry and also safe insulation. Building materials may also contain adhesives, fiber glass, wood and paper products. See specific protocols for those components. Additional instrumental analysis of FTIR may be utilized for building materials.

4.3.1.8.4. Paper match examinations (see Appendix III)

4.3.1.8.4.1. If a physical fit is not made or possible between a paper match to a book of matches, additional physical and chemical analysis can be completed. Match heads and/or match stems can be examined for physical characteristics including color, porosity, shape, wax line, measurements of width, length and thickness. In addition, the torn fibers can be compared as well as microscopical comparison of inert ingredients in the match head. Further chemical analysis can be completed by SEM-EDS, XRF and/or MSP.

4.3.1.8.5. Soil examinations (see Appendix IV)

4.3.1.8.5.1. Soils vary with respect to color and mineralogy. These variations can be used for differentiation. Soils can be complicated mixtures that also can include other trace evidence (e.g., paint chips, vegetative matter, and glass) that can also be examined. The gross color, sieve fractions, mineral content as well as



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 6 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

instrumental procedures can be utilized for soil comparisons. The same general methods for soil can be applied to certain aspects of building materials such as plaster, concrete, sheetrock, masonry and also safe insulation.

4.3.1.8.5.2. NOTE: Soil exams are not currently covered under the ANAB scope and therefore should be reported without using the ANAB logo

4.3.1.8.6. Wood examinations (see Appendix V)

4.3.1.8.6.1. The most reliable approach of identifying wood is based on its microscopic features. A low power microscopical examination (10-30X) of prepared wood samples can be used to classify wood as soft or hard wood, or if enough sample is present, to genus or species. The later classifications will require thin sectioning of the wood sample for examination via high power microscope (100-400X).

4.3.1.8.6.2. NOTE: Wood exams are not currently covered under the ANAB scope and therefore should be reported without using the ANAB logo

5. Quality Assurance and Controls

- 5.1. Appropriate controls, blanks and reference materials should be used for each test. Appropriate blanks, controls and calibrations / performance checks and adjustments will be employed per individual instrument protocols.
- 5.2. Microscopes, micrometers / measuring devices, and all scientific equipment should be properly calibrated or performance checked according to the protocols for each instrument (see *ATF-LS-E21 – Maintenance and Performance of Measuring Devices*)
- 5.3. The techniques described below for examination of general unknowns and uncommon evidence are all well-known and scientifically accepted in the forensic science community and in the relevant private industry of each material. Relevant examples of related literature can be found in Section 6 References.
- 5.4. Controls or standards are often not submitted with evidence. A similar store bought item may prove useful as a reference.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 7 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

5.5. For comparisons, the questioned item is evaluated to identify physical characteristics (e.g., color, layer structure, dimensions) suitable for comparison prior to examination of the known sample. Any subsequent chemical and elemental analysis of the unknown item shall be conducted prior to the known item. In certain circumstances, the known may need to be screened to determine a suitable analysis scheme for unusual evidence.

6. References

6.1 General unknown

Clarke's Isolation and Identification of Drugs, 2nd Edition, A.C. Moffat, ed. The Pharmaceutical Press, 1986.

Clinical Toxicology of Commercial Products, 4th Edition, Gosselin, Hodge, Smith, Gleason. The Williams & Wilkins Co, Baltimore, 1976.

"Detection of Some Non-Drug Poisons in Simulated Stomach Contents by Diffusion into Various Color Reagents," Stevens, H.M. Journal of the Forensic Science Society, 1986; 26:137-145.

The Quintessential Tinchorn – A Practical Guide to the Identification of Everything. Daley, I.P., 2006.

Food Additives Handbook, Richard J. Lewis. Von Nostrand Reinhold, New York, 1986.

Identification of Materials, A. A. Benedetti-Pichler. Springer-Verlag, New York.

Merck Index, 11th Edition, S. Budavari, ed. Merck and Co., Inc., 1989.

Organische Mikrochemische Analyse, Behrens-Kley. Microscope Publications, Chicago, 1969.

The Particle Atlas, 2nd Edition, McCrone and Delly. Ann Arbor Science, Ann Arbor MI, 1973.

The Pesticide Manual, 9th Edition, Charles R. Worthing, ed. British Crop Protection Council, Surrey, U.K. 1991.

"Characterization and Identification of Water Soluble Explosives" Thomas Hopen and John Kilborn, The Microscope, Vol 33, No. 1.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 8 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

“Extended use of Squaric Acid as a Reagent in Chemical Microscopy” by V. L. Whitman and W. F. Wills, Jr., The Microscopce, Vol. 25, No. 1.

Particle Atlas Vol. II. 2nd Edition, McCrone, W. & Delly, John, Ann Arbor Publications, 1973.

“Chemical, Clinico-Chemical Reactions, Tests and Reagents”, Fifth Edition, Merck Index, Merck & Co, 1940.

“Identification of General Unknowns”, Bowen, Andrew, Journal of the American Society of Trace Evidence Examiners, Vol. 1, Issue 1, pp 73-100.

6.2 Microchemical Tests

Handbook of Chemical Microscopy, 2nd Edition, Chamot and Mason. McCrone Research Institute, Chicago, 1989.

Spot Test Analysis-Clinical, Environmental, Forensic, and Geochemical Applications, Ervin Jungreis. John Wiley & Sons, 1986.

Spot Tests in Inorganic Analysis, 6th Edition, Fiegl and Anger. Elsevier, Amsterdam, 1972.

6.3 Bank Dyes and Lachrymators

Martz, R.M., Reutter, D.J. and Lasswell, L.D., “A Comparison of Ionization Techniques for Gas Chromatography/Mass Spectrometry Analysis of Dye and Lachrymator Residues from Exploding Bank Security Devices,” Journal of Forensic Sciences, Vol. 28, No. 1, Jan 1983, pp. 200-207.

Egan, J.M., Rickenbach, M., Mooney, K.E., Palenik, C.S., Golombeck, R., and Mueller, K.T. “Bank Security Dye Packs: Synthesis, Isolation, and Characterization of Chlorinated Products of Bleached 1-(methylamino)anthraquinone,” Journal of Forensic Sciences, Vol. 51, No. 6, Nov 2006, pp. 1276-1283.

FBI Bank Security Device Workshop, AAFS 57th Annual Meeting, February 22, 2005 (located on Burshare).

Fung, T., Jeffery, W. and Beveridge, A.D., “The Identification of Capsaicinoids in Tear-Gas Spray,” Journal of Forensic Sciences, Vol. 27, No. 4, Oct. 1982, pp 812-821.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 9 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

Gag, J.A. and Merck, N.F., "Concise Identifications of Commonly Encountered Tear Gasses," Journal of Forensic Sciences, Vol. 22, No. 2, April 1977, pp. 358-364.

Katoaka, M., et al, "Stability and Detectability of Lachrymators and their Degradation Products in Evidence Samples", Journal of Forensic Sciences, Vol. 47, No. 1, 2002, pp. 44-51.

Sreenivasan, V.R. and Boese, R.A., "Identification of Lachrymators," Journal of Forensic Sciences, Vol. 15, No. 3, July 1970, pp. 433-442.

Mongan, A. and Buel, E., "Identification of Dog Repellent in the Clothes of an Assault Suspect Using Gas Chromatography/Mass Spectrometry," Journal of Forensic Sciences, Vol. 40, No. 3, May 1995, pp. 513-514.

6.4 Building Materials

ASTM C 11 Standard Definitions of Terms Relating to Gypsum and Related Building Materials and Systems.

ASTM C 219 Standard Terminology Relating to Hydraulic Cement

ASTM C 51 Standard Definitions of Terms Relating to Lime and Limestone

McCrone, WC. Identification of Asbestos by Polarized Light Microscopy. The Microscope. Volume 25 Fourth Quarter 1977.

Microscopy of Building Materials, MAFS Workshop 2000

Miller ET. A Practical Method for the Comparison of Mineral Wool Insulations in the Forensic Laboratory. Journal of the AOAC, Vol. 58, No 5, 1975.

The Particle Atlas, 2nd Edition, McCrone and Delly. Ann Arbor Science, Ann Arbor MI, 1973.

6.5 Paper matches

Andrasko, J, "Identification of Burnt Matches by Scanning Electron Microscopy", JFS, 1978, Vol. 23, No. pp. 4637 – 642.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 10 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

Dixon, KC “Positive Identification of Torn Burned Matches with Emphasis on Cross Cut and Torn Fiber Comparisons”, *Journal of Forensic Sciences*, Vol 28, No. 2 April 1983, pp. 351-359.

Glattstein, B., Landau, E., and Zeichner, A., "Identification of match head residues in Post-Blast Debris", *JFS*, 1991, Vol. 36, No. 5, pp. 1360-1367

“Matches and Fireworks”, *Poor Man’s James Bond*, Vol. 1, pp. 453-473.

“Matches”, Herbert Ellern, PhD., *Military and Civilian Pyrotechnics*, Chemical Publishing Company, Inc., New York, 1986, pps. 65-83

6.6 Soil

Forensic Soil Analysis, Wehrenberg, John P., MAFS Workshop 1990.

MAFS Forensic Soils Workshop, Bisbing, Dick, et al, 2004

Forensic Examination of Soil, Murray, Raymond C., in *Richard Saferstein's Forensic Science Handbook*, Prentice-Hall 1982

Evidence from the Earth, Murry, Raymond C., Mountain Press Publishing 2004

6.7 Wood

Identifying Wood, Hoadley, Bruce, Taunton Press, Conn. 1990.

The Practical Identification of Wood Pulp Fibers, Parhum, Russell A. & Greg, Richard, L., Tappi Press, 1982.

“Identification of North American Commercial Pulpwoods and Pulp Fibers” Strelis and Kennedy, University of Toronto Press, 1967

“Key to Some Common U.S. Woods.” Trimpe, Mike, Introduction to Wood Identification Workshop, MAFS, 1996.

“Computer-Aided Wood Identification”. Wheeler, E. A., et al, North Carolina State University, 1986.

“Fiber Analysis of Paper and Paperboard” T401 om-88 Official standard from the Technical Association of the Pulp and Paper Industry (TAPPI), 1988.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 11 of 27
Original maintained by Quality Programs; copies are uncontrolled.	



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 12 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

APPENDIX I--Frequently Used Micro Chemical Tests

1. It should be noted that slight variations in the formulations of each of these reagents may be acceptable. Regardless, all chemical reagents should be tested on a known sample prior to each use in order to test the reliability of the reagent. When a reagent is made, the bottle shall be labeled with the name of the reagent and the date it was made or lot number at a minimum. Records shall be kept as to who made the reagent and that it was tested for reliability. The list below is not all inclusive, but any reagents or tests used in the laboratory shall be well documented in literature and generally accepted in the scientific community.

2. General Tests

2.1 10% HCl--acidify test sample with drops of dilute HCl. Gas evolution indicates bicarbonates, carbonates, cyanides, hypochlorites (bleach), nitrates or nitrites. Use caution as cyanide gas is very poisonous.

2.2 5% AgNO₃--precipitates many ions. Most precipitates are white.

2.3 5% BaCl₂--precipitates many ions. Most precipitates are white.

2.3.1 Precipitated by AgNO₃ and insoluble in HNO₃:

Iodide, I ⁻	Sulfide, S ⁻²
Bromide, Br ⁻	Cyanide, CN ⁻
Chloride, Cl ⁻	Thiocyanate, SCN ⁻
Hypochlorite, ClO ⁻	

2.3.2 Precipitated by AgNO₃ and soluble in HNO₃:

Cyanates, CNO ⁻	Boric acid, H ₃ BO ₃
Carbonic acid, H ₃ CO ₃	Iodic acid
Oxalic acid, C ₂ H ₂ O ₄	

2.3.3 Precipitated by AgNO₃ and BaCl₂; soluble in HNO₃:

Sulfites, SO ₃ ⁻²	Thiosulfates, S ₂ O ₃ ⁻²
Arsenite, As ⁺³ , As ₂ O ₃	Arsenate, As ⁺⁵ , AsO ₄ ⁻³
*Phosphate, PO ₄ ⁻³ yellow w/ AgNO ₃	Chromic acid
Carbonate, CO ₃ ⁻²	
Bicarbonate, HCO ₃ ⁻ cream w/ AgNO ₃	
*Silver nitrate does not precipitate phosphoric acid due to acidic medium	

2.3.4 Precipitated by BaCl₂ and insoluble in HNO₃:

-Sulfate, SO₄⁻² (high concentrations of sulfate can cause crystal formation with silver nitrate)



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 13 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

-Fluoride, F-

- 1.1 1% Diphenylamine/Concentrated Sulfuric Acid (fresh) -- blue color develops with the presence of the following oxidizers: chloride, bromide, iodide, chlorates, nitrates, nitrites, hypochlorite, bromate, iodate, permanganate, Fe^{+3} , Sb^{+5} , and peroxides. An immediate and permanent blue/purple indicates NO_3^- . A similar color is obtained with relatively concentrated solutions of FeCl_3 . Immediate blue colors are produced by ClO_3^- and NO_2 . but color from the latter fades rapidly and in about 1 minute is yellow green. At low levels, color development may occur after standing a short time. Similar reactions may also be observed with chloride, bromide, iodide, hypochlorite, bromate, iodate, permanganate, Fe^{+3} , Sb^{+5} , and peroxides.
- 1.2 Fujiwara Test--indicates presence of chloral hydrate, trichloroacetic acid, chloroform, bromoform, iodoform, and other compounds with at least two halogen atoms attached to one carbon. *Procedure:* to 1 ml of sample, add 1 ml 5N NaOH and 1 ml pyridine. Heat for two minutes in boiling water. Red or pink color in pyridine layer is positive.
- 1.3 Reinsch Test--indications for mercury, silver, arsenic, antimony and bismuth. *Procedure:* Add 3 ml conc. HCl to 15 ml sample. Immerse a copper wire that has been cleaned with concentrated HNO_3 in sample and heat gently ($80\text{-}90^\circ$) for 1 hour. Examine copper for discoloration every fifteen minutes. A silvery deposit is given by mercury and silver. A black deposit is given by bismuth and arsenic. A purple deposit is given by antimony.
- 1.4 5% Brucine Sulfate in H_2SO_4 --orange to red color indicates nitrates, nitrites or chlorates.
- 1.5 Sugar test--to a drop of sample or solid sample add 1 drop of 15% 1-naphthol in EtOH and then 3-4 drops of conc. sulfuric acid. If sucrose or fructose is present a blue to purple color will appear; if glucose or maltose is present a pink-red color will develop.
- 1.6 Metals by Ammonium sulfide--to a drop of liquid sample acidified with 5% HCl, add a drop of aqueous $(\text{NH}_4)_2\text{S}$. Perform tests in hood. Many **metal ions** give colored precipitates:
- 1.6.1 Black precipitate: indicates Hg, Pb, Ag, Bi, Cu, Co, Ni, or Fe. With addition of concentrated HCl: Bi dissolves; Pb turns grey; Fe turns rust colored or dissolves to orange solution.

Yellow precipitate and solution indicates Cd.

Dark brown precipitate indicates Sn.

Reddish-brown precipitate indicates Pt.

Peach precipitate and solution indicates Mn.

Orange precipitate indicates Sb.

Milky white precipitate indicates Zn. ZnS is soluble in excess $(\text{NH}_4)_2\text{S}$.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 14 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

3 Specific Tests

- 3.3 Ethchlorvynol--add crystals of diphenylamine to an alcoholic solution of the sample; slowly trickle in concentrated H_2SO_4 . Red color positive.
- 3.4 Thiocyanate (nitroprusside)--add drop of 5% ferric chloride. Red color is positive.
- 3.5 Cyanide--add two drops of concentrated H_2SO_4 to 2-3 drops sample in test tube. Cover top of tube with a cover slip with a hanging drop of $AgNO_3$; warm at $80^\circ C$ for 4-5 min. Search hanging drop for crystals of $AgCN$ --tiny, highly refractive, short rods or sheaves of slender needles. Rod's RI's $n^\wedge = 1.685$ and $n_{||} \gg 1.685$.
- 3.6 Arsenates--red precipitate with $AgNO_3$. View crystals with microscope.
- 3.7 Arsenites--yellow precipitate with $AgNO_3$. Best if ammoniacal $AgNO_3$ is used. Add concentrated ammonium hydroxide to 5% $AgNO_3$ until precipitate dissolves upon mixing. Add drop of this reagent to drop of sample. View crystals with microscope.
- 3.8 Oxalic acid, oxalate salts--to the acid or acid solution of the salt add drop of 10% ferrous sulfate. Yellow precipitate positive.
- 3.9 Lithium ion--add sample drop to glass slide and heat to dryness to remove any possible ammonium salts. Add drop of 15% hexamethylenetetramine (hexamine) to dried residue. Transfer this drop to another glass slide in two separate drops. To one drop add a crystal of $K_3Fe(CN)_6$ (potassium ferricyanide); to the other a crystal of $K_4Fe(CN)_6$ (potassium ferrocyanide). The ferricyanide yields yellow octahedra that appear birefringent due to high strain within the crystal; ferrocyanide yields short rods and radial clusters of rods. To help form the ferrocyanide crystals, push crust at edge of drop back into the middle and scratch slide with a glass rod. *Negative samples* of the ferricyanide also yield stars and yellow octahedra; however, these crystals are of *very low* birefringence.
- 3.10 Bleach containing Hypochlorite -- pH should be basic. Test with hanging drop of 5% silver nitrate by acidification with 5% HNO_3 . Wash and dry precipitate in reagent drop with distilled water and dissolve precipitate with drop of 50% ammonium hydroxide. Add coverslip and using PLM look for formation of highly refractive cubic crystals of silver chloride along edge of coverslip. This indicates the presence of chloride ion from evolution of Cl_2 from the test drop. Crystals are then confirmed as $AgCl$ via X-ray analysis.
- 3.11 Iodine Solution - Place a small amount of material on a microscope slide and cover with a cover slip. Add I_2 reagent and allow it to flow under the coverslip. Examine utilizing PLM.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 15 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

Starch grains and gelatinized starch particles stain purple/blue to red/brown. Color produced depends on the amylase content.

- 3.12 10% Povidone-Iodine (Betadine) Solution - Examine utilizing PLM. Starch grains and gelatinized starch particles stains purple/blue to red/brown. Color produced depends on the amylase content. Advantage of this test over the Iodine Solution is that that “Maltese” cross can be observed after the starch grains pick up the stain.
- 3.13 Fehling’s Test for Reducing and Non-Reducing Sugars – A material to be tested is gently heated to a boil in a drop or two of Fehling’s solution. If a reducing sugar (e.g. lactose, maltose, etc) is present, the solution will turn yellow/orange. For a non-reducing sugar, the solution will stay blue. To test for a non-reducing sugar (e.g. sucrose), warm the material to be tested in dilute HCl and then add the Fehling’s solution. The solution will turn yellow/orange if a non-reducing sugar was originally present.
- 3.14 Selleger’s Stain and Graff “C” for cellulose fibers – Add stain to paper fibers which have been disintegrated and dispersed on a microscope slide. Cellulose fibers will stain different colors depending on pulp make-up and previous chemical treatment.
- 3.15 Ammonia or Ammonium Ion -- precipitate using hanging drop of 10% platinum chloride by volatilizing ammonium ion to ammonia by adding 10% sodium hydroxide to test sample. To test for presence of ammonia gas (anhydrous ammonia) place drop of reagent on glass slide and place slide in airtight container with specimen. Allow to sit an appropriate amount of time (overnight if necessary) to allow for the formation of octahedral crystals indicative of the ammonium ion reaction product. Crystals thus formed can be rinsed with distilled water, dried and analyzed via IR spectroscopy.
- 3.16 Ethylene Glycol—See 4.3 Procedure above and/or consult a fire debris chemist.
- 3.17 Hydrogen Peroxide -- Use two tests.
- 3.17.4 Reduction test: Place one drop of 1.0% potassium ferricyanide/0.5% ferric chloride in spot well. Add test drop(s). Prussian blue coloration indicates hydrogen peroxide. Very dilute solutions may give a green coloration.
- 3.17.5 Oxidation test: Soak filter paper with 0.5% lead acetate. Hold over open bottle of 24% ammonium sulfide. Paper will become brown due to formation of PbS. Allow paper to dry. Spot paper with drop of sample. A white coloration indicates hydrogen peroxide. If only one of the tests is positive something other than hydrogen peroxide is indicated.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 16 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

APPENDIX II—Bank dyes and lachrymators

1. Identification of bank dyes

1.1 Examination of stained items

1.1.1 Note areas with bright red stains. Record physical properties applicable to the stain such as location on substrate, dimensions, pattern, etc. in the examination record.

1.1.1.1 NOTE: MAAQ is a fine powder and is easily distributed. Take care not to contaminate unstained areas during handling of evidence so as to maintain an area available for a comparison sample.

1.1.2 Remove a section of the evidence containing the stain. If available, remove a section of an unstained area as a comparison sample. If removal is not possible, swab the stained and unstained areas with separate swabs wet with methanol.

1.1.2.1 NOTE: Do not sample all of the stain if it is not necessary; a 1”x1” heavily stained area should be more than enough for analysis. If a garment has been laundered prior to submission, a comparison sample will not be possible, and the sample taken will have to be larger.

1.1.3 Wash the two sections or swabs with approximately 5 mL methanol into separate evaporating dishes. If using swabs, extract one unused swab as a control. Filter if necessary. Evaporate the washings down to a volume suitable for analysis (approximately 1 mL or until solution is bright red).

1.1.4 In a separate area, make up separate dilute reference samples.

1.1.4.1 Dilute the reference MAAQ in methanol, concentrated just enough to attain a bright red color.

1.1.4.2 Dilute (approximately 1% w/v) solutions of CN and/or CS reference materials in methanol.

1.1.5 Run a sample each of the unknown, the comparison sample (if available), the control (if needed), and the reference on GC-MS.

1.2 Examination of bleached items



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 17 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

- 1.2.1 Examine evidence. Note areas with faint red stains, bleached areas, or areas with damage or holes. Record physical properties applicable to the stain or damage such as location on substrate, dimensions, pattern, etc. in the examination record.
- 1.2.2 If possible, remove a section of the evidence containing the stain or damage. If removal is not possible, swab the area with swabs wet with methanol.
 - 1.2.2.1 NOTE: A comparison sample will probably not be available with bleached items
- 1.2.3 Wash the sample with methanol into a beaker. Filter the washing into an evaporating dish. Evaporate the washing down to a volume suitable for analysis (approximately 1 mL).
- 1.2.4 In a separate area, make up a dilute solution of chlorinated MAAQ derivatives:
 - 1.2.4.1 Place 5 mg of MAAQ into an Erlenmeyer flask with 5 mL methanol
 - 1.2.4.2 Add 20 mg of $\text{FeCl}_3 \cdot 6\text{H}_2\text{O}$ to the solution
 - 1.2.4.3 Add 700 μL of 7% sodium hypochlorite solution
 - 1.2.4.4 Allow the precipitate to settle, filter off the supernatant
 - 1.2.4.5 Set the precipitate to dry
 - 1.2.4.6 Place a small amount of the precipitate in methanol for analysis
- 1.2.5 In a separate area, make up a dilute solution of reference MAAQ in methanol, concentrated just enough to attain a bright red color.
- 1.2.6 Run a sample each of the unknown, the control (if needed), and the MAAQ and Cl-MAAQs references on GC-MS.

2. Identification of lachrymators

2.1. Examination of a substrate

- 2.1.1. Examine the evidence and note the presence of any stains. Employ alternative lighting as necessary. Record physical properties applicable to the stain such as location on substrate, dimensions, pattern, color, etc.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 18 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

2.1.2. If possible, remove a small section of the evidence containing the stain as well as an unstained area as a comparison. If removal is not possible, swab the stained and unstained areas with separate swabs wet with methanol.

2.1.2.1. NOTE: Do not sample all of the stain if it is not necessary; a 1"x1" heavily stained area should be more than enough for analysis. If a garment has been laundered prior to submission, a comparison sample will not be possible, and the sample taken will have to be larger.

2.1.3 Wash the sections or swabs with ~ 5 mL methanol in two separate evaporating dishes. If using swabs, extract one unused swab as a control. Filter if necessary.

2.1.4 Evaporate the washings down to a volume suitable for analysis - approximately 1 mL or until solution is dark orange.

2.1.5 In a separate area, prepare dilute (approximately 1% w/v) solutions of CN, CS, and/or capsaicin reference materials in methanol.

2.1.6 Run a sample each of the unknown, the comparison sample (if available), the control (if needed), and the reference materials on GC-MS.

2.2 Examination of a canister

2.2.1 Examine canister, noting brand, ingredients and volume/mass of contents according to label. If available, note serial number.

2.2.2 Record physical properties applicable to the sample such as solution morphology, color, etc.

2.2.3 Using a pipette, place one drop of the dispensed liquid into an auto-sampler vial. Fill the vial to the 1.5 mL mark with methanol, seal. If canister is empty, rinse interior with a minimal amount of methanol and place rinse into an auto-sampler vial.

2.2.4 In a separate area, prepare dilute (approximately 1% w/v) solutions of CN, CS, and capsaicin reference materials in methanol.

2.2.5 Run a sample each of the, the unknown, the comparison sample (if available), the control (if needed), and the reference materials on GC-MS.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 19 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

APPENDIX III – Paper Matches

1. Matchbooks are produced from paperboard which is finished and treated with an anti-afterglow solution. The paperboard rolls are cut into long strips called combs. These combs are then dipped into a wax, dried, and then dipped into the match-head solution and dried again. The head is mainly composed of potassium chlorate (oxidizer), sulfur (fuel) and glue with some inert ingredients. The standard match book will contain two combs of 10 stems, a total of 20 matches.
2. Physical characteristics
 - 2.1 Initially, the examination and comparison of matches is made by visual inspection including utilization of a stereo binocular microscope. Some features may only provide class characteristics, whereas others may be unique and provide individual characteristics. These features are as follows:
 - 2.1.1 Match Head
 - 2.1.1.1 The match head color, porosity, shape and size should be noted. Even burned heads may reveal this information.
 - 2.1.2 Stem color
 - 2.1.2.1 The front facing surface layer of the match stem frequently has a distinctly different color as compared to the underlying match stem body due to pigmentation and/or dying. Even the front surface of brown/tan stem matches can have a slightly different appearance than the interior of the match body. The use of a simple longwave UV lamp or alternate light source may also be employed during the examination of match stems which may provide additional comparative information.
 - 2.1.3 Wax line
 - 2.1.3.1 The wax on the match stem can normally be seen as a slight darker discoloration on the upper portion of the match stem. The depth of the wax line on the match stems can vary between books and within a book of matches.
 - 2.1.4 Stem width
 - 2.1.4.1 The width of matches usually fall into two groups; ones that have a width of approximately 3.3 mm and ones that have a width of



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 20 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

approximately 2.7 mm. The approximately 2.7 mm (specification is 0.0108 inches) width is a patented dimension and matches exhibiting this width are only manufactured by D. D. Bean & Sons (3). However, it must be noted that this does not mean that the matchbook will have “D. D. Bean & Sons” markings on the match cover since D. D. Bean & Sons produces matches with this dimension for other companies and other companies produce matches other than 2.7 mm for D.D. Bean & Sons.

2.1.5 Stem length and thickness

2.1.5.1 The match stem length, when placed at the cardboard base of the matchbook should correspond to the length of the known unburned matches in the matchbook. If the match is burned, a portion of the head must still be present to conduct an accurate comparison. The match thickness does not vary much and cannot be related to a particular manufacturer.

2.1.6 Base stem cut/indent

2.1.6.1 Some matchbooks may be cut or have an indentation at the base of the match stem to aid in removal of the match from the matchbook. The cut/indent may be consistent on every match or vary within a book.

2.1.7 Cut edge abnormalities

2.1.7.1 Cut edge abnormalities appear along the vertical edge of the match body as small irregular cuts or tears. These imperfections are due to a cutting blade becoming dull over time and are another potential point of comparison to an adjacent match in a book.

2.1.8 Cross cut and torn fibers

2.1.8.1 Cross cut and torn fibers may provide unique comparable features that can associate a match to a particular matchbook. Cross cut (horizontal) and torn (vertical) fibers are noted as darker colored fibers contrasted against the more lightly colored fibers. Cross cut (horizontal) and torn (vertical) fibers are recognized under low magnification utilizing a stereomicroscope. The horizontal fibers are fibers which cross individual match stems and have been cut during the manufacturing process. Vertical fibers are the contrasting fibers which run from the base into the match stem and are torn in two when the match is removed from the book. Torn fibers are less useful when attempting to make a positive association since



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 21 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

the tearing action of the match from the cardboard base may distort any comparison. Many times the vertical fibers may not be torn in two but are completely pulled from the base or stem when the match is removed. One can increase the contrast between the fibers in the match stems by use of stains but it should be noted that the use of stains may permanently alter the color of the match stems. One simple way to increase the contrast between fibers is to place a droplet of an 80:20 deionized water: ethanol on the match stems, allow it to set for a moment, and then wick off any excess liquid.

2.1.9 Inclusions

2.1.9.1 Foreign matter inclusions are common artifacts in match stems and many times are cut in two when adjacent stems are cut by the blade.

3. Analytical techniques

3.1 PLM

3.1.1 Some of the common inert ingredients that may be present in the match head that can be quickly identified by PLM include quartz (irregular grains, $\omega = 1.544$ and $\epsilon = 1.553$), glass fragments (irregular chips, $n \sim 1.52$), diatoms ($n \sim 1.44$ with very fine structure), and wollastonite (fibrous, $\alpha \sim 1.62$, $\beta \sim 1.63$, $\gamma \sim 1.64$). Pigments and starch grains may also be noted during a PLM examination. The presence or absence of any constituent may provide quick differentiation. Also, it helps if one removes the water soluble components with warm water using micro extraction techniques. Pigments and inclusions in stems can also be characterized by PLM.

3.1.2 Potential analysis of fibers in the match paperboard by differential staining has been reported (Dixon) however this is a destructive method. Refer to references for further detail for the following stains:

3.1.2.1 Herzberg and Selleger's stains

3.1.2.2 Graff "C" stain

3.1.2.3 Green and Yorston stain

3.2 SEM-EDS



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 22 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

3.2.1 SEM-EDS can provide bulk elemental information and can also be employed to characterize and identify particulate material, pigments and inclusions as well as can confirm the constituents identified by PLM.

3.3 XRF

3.3.1 Samples should be analyzed using a 40 KeV excitation energy to allow heavier elements such as strontium (Sr) and zirconium (Zr) to be detected. Spectra of the match heads and for stems can be completed.

3.4 MSP

3.4.1 Transmission or reflectance can be utilized. Red match heads have been shown to be differentiated by this technique.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 23 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

APPENDIX IV – Soil

Soil exams are not currently covered under the ANAB scope and therefore should be reported without using the ANAB logo

1. Additional information on soils, mineralogy and building materials is on file in the trace evidence section. The same general methods for soil can be applied to certain aspects of building materials such as plaster, concrete, sheetrock and masonry and also safe insulation. When possible, known soil and/or building materials should be collected and submitted for comparison purposes.
2. Initial color and gross composition
 - 2.1. A visual examination is first conducted to see if the soil samples are similar in color and gross composition. If the soil samples are not dry they can be dried in an oven for several hours or overnight. Visually compare color of dry soils.
 - 2.2. Initial color
 - 2.2.1. Place similar amounts of the dried soil samples on a watch glass or other suitable glassware and evaluate the samples for color. Also, the soil samples may be moistened and the color of the damp soil samples compared. If differences in color are observed, the examination may be complete. In addition, the soil may be compared and classified using Munsell color charts if desired.
 - 2.3. Gross composition
 - 2.3.1. Examine each sample under the stereoscope to determine if the gross composition is similar or different between the control and questioned soils. Note presence of man-made materials such as glass, brick, paint or fibers that may also be useful for comparison purposes.
3. Sieving, pH and turbidity
 - 3.1. If sample size allows for calculation of fraction sizes, the examiner may weigh the amount of soil to be sieved. Large clumps may be broken up by mortar, rubber mallet, gloved hands, glass rod or sonication.
 - 3.2. Place soil samples in a beaker and add distilled water. Turbidity and the amount of floating organic debris may be noted. Check pH if desired.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 24 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

- 3.3. Wet or dry sieve using a set of mesh sieves and collect the silt fraction in the pan or filter paper. Collect fractions and dry.
 - 3.4. Compare colors of the soil samples of like sized mesh sizes. The examiner may calculate the weight percent of each fraction to the total original weight and record. Soil samples with a common origin should have similar weight fractions; however, questioned samples may have lost all or some of the larger sized fractions, i.e., soil from pants may be primarily small particle sized or clay.
4. Soil separation and Polarized Light Microscopy
 - 4.1. Select the sieve fraction of grains in the 150 mesh sieve to clean for PLM.
 - 4.1.1. Place an aliquot in test tube and add 2 mL distilled water.
 - 4.1.2. Sonicate, allow to settle for several seconds and draw off turbid slurry. Repeat until the supernate is clear. Wash with acetone.
 - 4.1.3. Add bromoform and gently shake. Centrifuge and allow to sit for a few minutes.
 - 4.1.4. Freeze the bottom half with liquid nitrogen. This portion contains the Heavy Mineral Fraction (HMF). Wash out the top half which contains the Light Mineral Fraction (LMF) into a clean test tube with acetone.
 - 4.1.5. Allow grains to settle and draw off the liquid and discard. Wash with acetone several times to remove all bromoform. Wash the HMF in the same manner.
 - 4.2. The HMF and LMF can be mounted and examined by PLM using Cargille liquids (light fractions are generally examined using 1.550 HD or 1.545 HD; heavy minerals are examined in 1.660). The examiner may record the number and types of minerals present. If a large amount of organic matter is present, it can be removed by adding 30% hydrogen peroxide. The number and type of minerals should be similar for soils with a common origin. The density of bromoform is 2.89 at 20 C°.
 - 4.2.1. Floats in bromoform (Light Mineral fraction)
 - 4.2.1.1. Quartz (2.65), Feldspars (2.5-2.8), Calcite (2.7), Opal (2.2)
 - 4.2.2. Sinks or floats
 - 4.2.2.1. Dolomite (2.8-2.9), Micas (2.76-3.4)



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 25 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

4.2.3. Sinks in bromoform (Heavy Mineral Fraction)

4.2.3.1. Amphiboles (2.9-3.5), Pyroxenes (3.3-3.6), Epidote (3.25-3.5), Olivine (3.27-3.37), Chlorite (2.6-3.0), Apatite (3.2), Limonite (3.8), Hematite (5.2), Magnetite (5.17), Garnet (3.8), Zircon (4.7), Tourmaline (2.9-3.2), Rutile (4.18-4.25), Staurolite (3.65-3.77), Corundum (3.95-4.10), Sillimanite (3.25), Kyanite (3.6)

5. Instrumental Methods

5.1. A variety of instruments such as SEM-EDS, XRF and XRD may be utilized in order to further identify or compare portions of the soil samples. Some building materials may also be analyzed by FTIR.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 26 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

APPENDIX V - Wood

Wood exams are not currently covered under the ANAB scope and therefore should be reported without using the ANAB logo

1. In order to microscopically identify wood as a softwood or a hardwood, thin transparent sections can be cut and mounted from “bulk” samples. Characteristics found within these sections are used to identify a sample of wood as hardwood or softwood. Determine if the piece of wood is large enough for stereomicroscopic examination and thin sectioning. If not, only a microscopical examination of wood fibers can be performed.
2. Wood fibers
 - 2.1 If only wood fibers are to be examined a stain such as Safrinin may be used and the sample can be mounted in an appropriate mounting medium. Examine using a high powered microscope. Look for microscopical characteristics, if present, that will allow classification of fibers as hard or soft wood; and, if appropriate, mechanically or chemically pulped. Some characteristic features may be present to determine a more specific classification.
 - 2.1.1 Softwoods are also known as Gymnosperms or conifers.
 - 2.1.1.1 There are microscopic features that may be observed in mounted cross-sections that are characteristic of softwoods.
 - 2.1.1.2 Cross section - Resin canals, rays, and tracheids.
 - 2.1.1.3 Radial section - Bordered pits, tracheids.
 - 2.1.1.4 Tangential section - Ray (fusiform with resin canal and uniseriate) and radial walls of vertical tracheids.
 - 2.1.2 Hardwoods are also known as dicots or broad-leaved.
 - 2.1.2.1 There are microscopic features observed in mounted cross-sections that are characteristic of hardwoods.
 - 2.1.2.2 Cross section - Rays and vessels.
 - 2.1.2.3 Radial section - Squared ended parenchyma, vessel elements, and rays.
 - 2.1.2.4 Tangential section - Boat-shaped rays, vessel elements, and square ended parenchyma.



ATF-LS-TE14 Examination of General Unknowns and Uncommon Evidence	ID: 1933 Revision: 5
Authority: Technical Leader	Page: 27 of 27
Original maintained by Quality Programs; copies are uncontrolled.	

3. Wood fragments

3.1 For larger wood fragments, razor cuts are made on the whetted wood to obtain either a clean cross-sectional surface for stereoscopic examinations, or thin sections for high power microscopic examinations. Thin sections from the cross-sectional, radial and tangential are made, if possible.



x - Cross section – a section cut perpendicular to the grain

t - Tangential section – a section cut along the grain that is more or less parallel to the growth layer

r - Radial section – a section cut along the grain that is perpendicular to the grain direction

3.2 Cross-sectional surfaces are examined via low power microscopy and keyed according to Hoadley, Trimpe (MAFS) key and/or other suitable keys. Document the source of the key(s) used in case records. Comparison to standard wood blocks can be helpful.

3.3 Thin sections may be treated with a stain such as Safranin and mounted in an appropriate mounting medium between slide and cover slip. The preparation may be heated to remove air bubbles. Examine sections via high power microscope. Samples are classified according to Hoadley, Trimpe (MAFS) key and/or other suitable keys. Document the source of the key(s) used in case records. Comparison to the thin section standards can be helpful.

4. Report results to the appropriate level of classification



ATF-LS-TE15-Examination, Analysis, and Comparison of Paint	ID: 1934 Revision: 5
Authority: Technical Leader	Page: 1 of 8
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

- 1.1. Many different types of crimes may involve situations where paint is transferred from one object to another or where paint is sprayed or applied to an object which is submitted as evidence. In these cases, the forensic paint examiner is commonly asked to compare questioned and known (Q and K) paint samples based on their physical and chemical compositions. In conducting those comparisons, the forensic paint examiner's goal is to assess the significance of any differences observed. The absence of any exclusionary differences between the known and questioned samples suggests that the paints could have had a common source of origin. Besides a Q vs. K comparison, the examiner may also be requested to analyze a questioned paint and attempt to determine the possible source(s) of origin for that sample.
- 1.2. The physical, optical, and chemical properties of known and/or questioned paints may include Physical - color, layering, microscopic properties, and surface characteristics. Chemical composition may be determined and compared by micro-solubility/micro-chemical tests, FTIR, SEM-EDS, XRD, XRF and PGC-MS.
- 1.3. In rare instances, a paint chip may be physically matched to a source. In this case a positive identification of the origin of the chip can be determined (Refer to *ATF-LS-TE10* Physical Match protocol).
- 1.4. Reference(s) to applicable OSAC Registry documents
 - 1.4.1. ASTM E1610 Standard Guide for Forensic Paint Analysis and Comparison

2. Instrumentation/Reagents

- 2.1. Scraping utensils
- 2.2. Tweezers, scalpel, and other appropriate tools
- 2.3. Clean butcher or Kraft paper
- 2.4. Evidence containers
- 2.5. Biohazard safety equipment (if necessary)
- 2.6. Vacuum and vacuum filters
- 2.7. Spot plates/microscope slides



ATF-LS-TE15-Examination, Analysis, and Comparison of Paint	ID: 1934 Revision: 5
Authority: Technical Leader	Page: 2 of 8
Original maintained by Quality Programs; copies are uncontrolled.	

2.8. Temporary or permanent mounting media

2.9. Appropriate solvents and micro-chemical test reagents (acetone, chloroform, etc)

2.10. Microtome and embedding medium

2.11. Microscopes

2.11.1. Polarized light microscope

2.11.2. Stereomicroscope

2.12. Camera or other Imaging Equipment

2.13. Instrumentation

2.13.1. FTIR (*ATF-LS-E6*)

2.13.2. MSP (*ATF-LS-TE03*)

2.13.3. Pyrolysis GC-MS or High Temperature GC-MS (*ATF-LS-TE04 / ATF-LS-FD2*)

2.13.4. XRD (*ATF-LS-E5*)

2.13.5. XRF (*ATF-LS-E4*)

2.13.6. SEM-EDS (*ATF-LS-E3*)

3. Safety Considerations

3.1. The examiner should follow all the biohazard procedures and use universal safety.

3.2. Precautions need to be taken whenever working with chemicals which could pose potential health hazards.

3.3. Precautions need to be taken when using sharp objects.

4. Procedure or Analysis



ATF-LS-TE15-Examination, Analysis, and Comparison of Paint	ID: 1934 Revision: 5
Authority: Technical Leader	Page: 3 of 8
Original maintained by Quality Programs; copies are uncontrolled.	

4.1. Paint Recovery Techniques

4.1.1. Purpose

4.1.1.1. To collect questioned paint samples from items of evidence.

4.1.2. Minimum standards and controls

4.1.2.1. When the paint is recovered by scraping or vacuuming, or the paint fragments are in debris, the examiner must clean the examination area and change the examination paper (using separate examination areas if possible) between victim and suspect or scene exhibits. The examiner will change the paper between items from the victim and the suspect or more often when appropriate.

4.1.2.2. The examiner must clean their tools between examining the evidence from the victim and the evidence from the suspect, or between examining evidence from different locations/scenes.

4.1.3. Representative sample

4.1.3.1. Some items may have too many paint chips or smears present on them to collect all paint present. Care shall be taken to select a representative sample of each visually different paint type for further analysis.

4.1.4. Analytical Procedure for recovery of questioned paint samples

4.1.4.1. Thoroughly clean the examination area and cover the worktable with new paper prior to conducting examinations between questioned and known items.

4.1.4.2. Remove the item of evidence from its packaging being sure to collect any loose paint chips that may be left in the packaging container.

4.1.4.3. Conduct a thorough inspection of the questioned item for any paint particles/deposits. Paint samples collected from different areas should be packaged separately and labeled appropriately. If possible, representative paint samples should be isolated using forceps and/or needles.

4.1.4.4. Garments and cloth items may be scraped or vacuumed to dislodge any adhering paint fragments. Scraping is done by holding or suspending the item over a clean sheet of paper and scraping the evidence thoroughly



ATF-LS-TE15-Examination, Analysis, and Comparison of Paint	ID: 1934 Revision: 5
Authority: Technical Leader	Page: 4 of 8
Original maintained by Quality Programs; copies are uncontrolled.	

using a clean spatula. If vacuuming is used, then separate filters should be used for different areas. Any recovered debris is collected in an evidence container for further analysis. As necessary, the evidence should be properly documented to include sketching, photography, and note taking, where appropriate, being sure to note paint deposits/smears and other unusual feature(s).

4.2. Stereomicroscope / PLM Examination

4.2.1. Purpose

- 4.2.1.1. To examine submitted paint evidence on a macroscopic and microscopic scale noting physical properties to assist in comparing known and questioned paint samples

4.2.2. Minimum standards and controls

- 4.2.2.1. All tools and work areas must be cleaned prior to beginning work and between samples from different locations.

4.2.3. Analytical Procedure for recovery of questioned paint samples

- 4.2.3.1. The sample is placed under the microscope and examined. The physical properties of each paint sample are noted and recorded on a worksheet or written notes. The layer sequence, color, texture, relative thickness of the layers and any unusual features should be noted.
- 4.2.3.2. If multiple layers are suspected, a thin peel, cross section, or bevel cut should be prepared to visualize the layers. If a cross section is made, it may be hand sectioned or mounted in an appropriate mounting media and sectioned using a microtome for subsequent analysis. The layer sequence, color, texture, thickness of the layers, pigment morphology, and any unusual features should be noted. If possible, pigment types should be identified. Comparison of the layers may require a comparison microscope.
- 4.2.3.3. If any exclusionary differences are observed between the known and questioned samples, the samples are dissimilar.

4.2.4. Sample selection



ATF-LS-TE15-Examination, Analysis, and Comparison of Paint	ID: 1934 Revision: 5
Authority: Technical Leader	Page: 5 of 8
Original maintained by Quality Programs; copies are uncontrolled.	

4.2.4.1. If a number of questioned paint chips are recovered, they shall be examined using the stereomicroscope and/or polarizing light microscope. If it is concluded that all the questioned paints are consistent in appearance (color, layering, and microscopic characteristics) to one another, additional analysis (e.g., micro-chemical tests, FTIR, SEM-EDS, MSP, PyGC-MS) can then be performed on a select few of the questioned paints. The report should be clear that the results are based only on the portion(s) tested.

4.3. Solvent / Microchemical Tests

4.3.1. Purpose

4.3.1.1. Determine the solubility and chemical reactivity of individual paint layers in known and questioned samples.

4.3.2. Minimum standards and controls

4.3.2.1. Solvents and chemical reagents are prepared and documented according to generally accepted recipes. Chemicals shall be checked on known samples or in some manner that assures they are working properly, and these checks shall be documented in the case record.

4.3.3. Analytical Procedure for recovery of questioned paint samples

4.3.3.1. Place the paint sample on a microscope slide or spot plate.

4.3.3.2. Apply the reagent or solvent and observe as it comes into contact with the sample. Any resulting reaction should be recorded. Note the effect of each reagent on the individual paint layers for the questioned and known paints. Use of a stereomicroscope will aid in the observation of any reaction.

4.3.3.3. The samples are dissimilar if any exclusionary differences are observed between the questioned and known paints. If samples have been subjected to different conditions (e.g. age, weathering, burning) caution should be used when interpreting differences and additional testing may be needed to confirm an exclusion.

4.4. Instrumental Analysis

4.4.1. Purpose



ATF-LS-TE15-Examination, Analysis, and Comparison of Paint	ID: 1934 Revision: 5
Authority: Technical Leader	Page: 6 of 8
Original maintained by Quality Programs; copies are uncontrolled.	

4.4.1.1. Other analytical instruments that may be employed to characterize organic and inorganic constituents are listed above (Section 2. Instrumentation//Reagents). These techniques are used to further discriminate between paints, as well as to provide classification and source assessment.

4.4.2. Minimum standards and controls

4.4.2.1. Reference data of known paints, pigments, and polymers from the instruments employed is available.

4.4.3. Analytical Procedure

4.4.3.1. Appropriate sample preparation and analytical parameters shall be used for each instrument used (see protocols for each instrument listed above).

4.4.3.2. When comparing paint samples, the same analytical techniques (i.e.: FTIR) should be performed in the same manner (i.e.: thin peel of each layer placed on a KBr pellet for analysis) on both the known and questioned paints.

4.4.3.3. During the paint examination scheme, if any exclusionary differences are detected between the questioned and known paint, a conclusion can be made that the paints do not have a common origin.

4.4.3.4. Generally, when sample size is limited, destructive testing is performed after all non-destructive testing is complete.

4.4.3.5. Compare the generated spectra/chromatograms of the known and questioned samples and evaluate the data.

4.4.4. It should be noted that due to the condition, size and/or type of paint, analysis using some of the aforementioned instrumentation may not be appropriate or possible.

5. Quality Assurance and Controls

5.1. Through proper training, competency testing, and proficiency testing of paint examiners as well as through the use of high quality equipment, which is appropriately cleaned,



ATF-LS-TE15-Examination, Analysis, and Comparison of Paint	ID: 1934 Revision: 5
Authority: Technical Leader	Page: 7 of 8
Original maintained by Quality Programs; copies are uncontrolled.	

maintained, and quality checked (e.g. calibrated, performance checked) and the laboratory's technical review process, the quality of this method is assured.

- 5.2. Because paints are mass produced, short of a physical match, a questioned paint cannot be positively identified back to a specific source; therefore, the use of error rates is not applicable.
- 5.3. Instruments used must be tuned and performance checked and adjusted as applicable. Appropriate standards, controls, and blanks will be utilized as needed per each instrumental protocol.
- 5.4. Validation
 - 5.4.1. The techniques described above for paint examinations are well known and scientifically accepted in the forensic community and in private industry. Relevant examples of related literature can be found in Section 6 (References).

6. References

6.1. ASTM International Standards

ASTM E2808 Standard Guide for Microspectrophotometry and color Measurement in Forensic Paint Analysis

ASTM E2809 Standard Guide for Using Scanning Electron Microscopy/X-ray Spectrometry in Forensic Paint Examinations

ASTM E2937 Standard Guide for Using Infrared Spectroscopy in Forensic Paint Examinations

E3234 Standard Practice for a Forensic Paint Analysis Training Program

- 6.2. Scientific Working Group for Materials (SWGMAT) Documents available at: www.asteetrace.org

SWGMAT Guide for Using Pyrolysis Gas Chromatography and Pyrolysis Gas Chromatography-Mass Spectrometry in Forensic Paint Examinations

6.3. Other



ATF-LS-TE15-Examination, Analysis, and Comparison of Paint	ID: 1934 Revision: 5
Authority: Technical Leader	Page: 8 of 8
Original maintained by Quality Programs; copies are uncontrolled.	

Beam TL, Willis WV. Analysis Protocol for Discrimination of Automotive Paints by SEM-EDX Using Beam Alignment by Current Centering. Journal of Forensic Sciences, Vol 35 (5), 1990, pp. 1055-1063.

Caddy B, ed. Forensic Examination of Glass and Paint: Analysis and Interpretation, Taylor and Francis, New York, NY, 2001.

Cardosi PJ. Pyrolysis-Gas Chromatographic Examination of Paints. Journal of Forensic Sciences, Vol 27 (3), 1982, pp. 695-707.

Levy EJ. The Analysis of Automotive Paints by Pyrolysis Gas Chromatography, Analytical Pyrolysis, 1977, pp. 319-335.

Linde HG, Stone RP. Application of the LeRosen Test to Paint Analysis. Journal of Forensic Sciences, Vol 24 (3), 1979, pp. 650-655.

McCrone, McCrone and Delly. Polarized Light Microscopy, Research Institute, 2001.

Ryland ST. Infrared Microspectroscopy of forensic paint evidence. In: Practical Guide to Infrared Microspectroscopy. Humecki, H. (ed.). Marcel Dekker, New York, 1995, pp 163-243.

Ryland ST, Jergovich TA, Kirkbride KP. Current Trends in Forensic Paint Examination. Forensic Sci Rev 18:97; 2006.

Thornton JI, Kraus S, Lerner B, Kahane D. Solubility Characterization of Automotive Paints. Journal of Forensic Sciences, Vol 28 (4), 1983, pp. 1004-1007.

Thornton, JI, Forensic Paint Examination. In: Forensic Science Handbook, Vol 1, Saferstein R., Ed. Prentice-Hall, Inc., 1982, pages 529-567.

Wright DM, Bradley MJ, Mehlretter AH. Analysis and Discrimination of Architectural Paint Samples via a Population Study, Forensic Science International, Vol 209, 2011, pp. 86-95.



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 1 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

1. Scope

1.1. This document describes the information that is included in trace evidence laboratory reports regarding the interpretation and reporting of the overall conclusion(s) for trace evidence examinations.

1.1.1 This document provides interpretation of evidence and example report wording for conclusions based on the most common types of trace examinations but can be applied to other trace materials. This document does not contain all possible examples, case circumstances, or all types of evidence that can be examined.

1.1.2 Reports should use wording similar to that described below, but alterations may be needed for specific cases. Alterations could include using a table, bullet points, or different wording. A report will include the justification for the conclusion reached and, where applicable, any limitations, caveats, or available techniques not used. If an applicable example is not listed below, one should be used that is most similar to the exams being performed or most appropriate.

2. General

When writing a report, the examiner shall interpret and report the overall meaning of the findings of the examinations, including any additional significance or limitations. For trace evidence comparisons, a qualitative approach to communicate the significance of an association or exclusion is used and based on a) the foundational validity of the scientific methods used for the comparison of the items, b) discrimination capabilities of the analytical protocol, and c) existing knowledge of how discriminating the compared characteristics are based on survey studies, reference collections, industry or manufacturing knowledge, and/or databases. This approach focuses primarily on fibers, paint, and tape but can be applied to other trace materials. A review article¹ provides a thorough bibliography that also serves as the body of work supporting the approach presented throughout this procedure for the interpretation of trace comparisons.

3. Types of analysis

3.1. Characterization Analysis

The following terminology is used in the reporting of trace material characterization examinations.

3.1.1 Specific terminology

¹ Trejos T, Koch S, Mehlretter A. Scientific foundations and current state of trace evidence – a review. *Forensic Chemistry*, 18, May 2020.



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 2 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

- 3.1.1.1. **Identification** – The analytical data provides reliable information to specify a particular chemical or product or contains specific characteristics that compare to a known standard or reference collection material which ensures its identification (e.g., acrylic fiber, human hair, OEM paint). The phrases “identified”, “were determined”, and “was deemed” are used in this context.
- 3.1.1.2. **Classification** – When a known standard or a reference collection material is not available or the evidence lacks quantity, quality, and/or detail to support an identification of a specific chemical, product, or species. (e.g., European head hair, spray paint, type of fabric damage). The phrase “consistent with” is used in this context.
- 3.1.1.3. **Indication** – The analytical data suggests a particular type of material but does not support a classification or identification. The terms “possible” and “similar to” are used in this context.
- 3.1.1.4. **Apparent** – Used when no analysis has been done to identify the specific material and/or the scientist is not trained to identify it. (e.g., blood, ridge detail)

3.1.2 Hair non-comparison examinations:

- 3.1.2.1 If human hairs are reported, the following storage statement must be included in the report.

Note: The human hairs in Exhibit X may contain biological evidence subject to specific storage and preservation requirements. Please reference the current version of ATF O 3400.1 to review the storage and preservation requirements of this evidence for the purposes of possible future DNA analysis.

- 3.1.2.2 An ancestry/body origin disclaimer, similar to the one below, should be added to reports that classify human hairs.

All ancestral and body area conclusions are based on the microscopic characteristics observed and their consistency with characteristics expected for a particular ancestral group or body area. How an individual identifies their ancestry may not correlate with the determinations made here.



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 3 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Hairs are typically classified as follows.

Ancestry:

African

European (including individuals of Middle Eastern descent)

Asian (including Native Americans)

Mixed (exhibits characteristics of more than one ancestral group)

Undetermined

Note: Hairs from individuals of Latin American origin may exhibit microscopic characteristics of one or more ancestral groups listed above.

Body Origin:

Head

Pubic

Body (more specific classification may be made)

Undetermined

3.2. Comparison Analysis

The following terminology is used in the reporting of trace material comparative examinations. The interpretation scale is utilized to demonstrate the significance of the conclusion.

3.2.1 Interpretation Scale

The following italicized wording is included as an appendix in the report of comparative exams with the exception of when only an “exclusion” conclusion is reached. In this instance, only the “exclusion” wording is necessary in the report.

The following descriptions are meant to provide context to the opinions reached in this report. Not every type of conclusion may be applicable in every case or for every material type.

Type I Inclusion: Source Identification – *Source Identification is the highest degree of association between items. This association provides the strongest support that the items originated from the same source as opposed to different sources. Source Identification, which includes a physical fit, is reached when the items display physical features that correspond/re-align in a manner that is not expected to be replicated.*

Type II Inclusion: Inclusion with Highly Discriminating Characteristics –



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 4 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

This is the highest degree of association that can be determined in the absence of a Source Identification. This type of association provides strong support that the items originated from the same source as opposed to different sources. The items correspond in all measured physical properties, chemical composition and/or microscopic characteristics and share highly discriminating characteristic(s) that would rarely be expected to occur in the relevant types of materials examined.

Type III Inclusion: Inclusion with Discriminating Characteristics – This type of association provides support that the items originated from the same source as opposed to different sources. The items correspond in all measured physical properties, chemical composition and/or microscopic characteristics; however, other items have been manufactured or could occur in nature that would also be indistinguishable from the examined materials.

Type IV Inclusion: Inclusion with Limitations – This type of association provides limited support that the items originated from the same source as opposed to different sources. Therefore, the possibility that the items came from the same source cannot be eliminated. As compared to the categories above, this type of association has decreased evidential value due to limiting factors such as the items are more commonly encountered, a limited analytical scheme was conducted, or minor variations were observed in the data.

Inconclusive – No conclusion could be reached regarding an inclusion or an exclusion between the items.

Exclusion with Limitations – This conclusion provides support that the items originated from different sources as opposed to the same source due to observed differences; however, an Exclusion conclusion was not reached due to limiting factors such as possible natural or manufactured source variations, damage or contamination that cannot be removed or avoided.

Exclusion – The items display differences that support that the two items did not originate from the same source.

4. Interpretation of evidence

The following are examples of how the interpretation scale is applied to specific types of evidence.

4.1 Fabric damage

Type I Inclusion: Source Identification

Not applicable to fabric damage examinations. See Fibers for fabric comparisons.



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 5 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Type II Inclusion: Inclusion with highly discriminating characteristics

It is unlikely this association could be used for fabric damage examinations

Type III Inclusion: Inclusion with discriminating characteristics

Damage consistent with an implement that has measurable class characteristics

- Pinking shears or dimensions of hole correspond with knife

Type IV Inclusion: Inclusion with limitations

Lack of distinguishing features in the damage produced by these implements and the inability to distinguish the cuts made from one type of implement from another

- Common scissors

Inconclusive

Damage due to a lack of features recorded or changes to the damage after it was made (melting, unraveling, stretching, etc.)

Exclusion with Limitations

The questioned item exhibits some dissimilarities to the known item but lacks sufficient quality or detail for an absolute exclusion to be made

Exclusion

Damage is different from that produced with an implement. For instance, damage on the shirt is consistent with coming from a knife and a comparison implement is a scissor

The mechanism which caused the damage could also be different (e.g., a cut vs a tear)

4.2. Fabric impressions

Type I Inclusion: Source Identification

Items share a combination of class characteristics and randomly acquired characteristics that demonstrates the questioned impression(s) were made by the known item

Type II Inclusion: Inclusion with highly discriminating characteristics

Some distinctive characteristics

- Officer's badge, a ragged hole, a patch

Type III Inclusion: Inclusion with discriminating characteristics

Items correspond in all class characteristics.

Common construction (twill pattern) with seams, unusual construction patterns, airbag singe patterns designating driver or passenger side airbag

Type IV Inclusion: Inclusion with limitations

Limiting factors in the impression or photograph

- Scale is not present or 1:1

Common construction (twill pattern in blue jeans)

Inconclusive

Interference from substrate

Limited sample size



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 6 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Lack of characteristics

Exclusion with Limitations

The questioned impression exhibits some dissimilarities to the known exhibit but lacks sufficient quality or detail.

Exclusion

Differences in pattern or spacing

4.3. Fibers

Type I Inclusion: Source Identification

Not applicable to single fibers, only applicable to fabric. The items exhibit physical features that demonstrate they were once part of the same object.

Type II Inclusion: Inclusion with highly discriminating characteristics

Questioned and known fibers have corresponding surface contamination or post-manufacturing marks such as staining or corresponding damage

Conditions that limit the possible sources of the fibers (e.g., fibers found in a vehicle with a limited number of passengers wearing known garments and only correspond to one garment)

Type III Inclusion: Inclusion with discriminating characteristics

Samples correspond in all chemical and physical characteristics with typical analytical scheme

- Questioned colored nylon fiber corresponding to a known carpet

Type IV Inclusion: Inclusion with limitations

Commonly observed fiber/fabric type (white cotton, blue denim cotton)

Limited characteristics to differentiate among fibers (colorless polyester or undyed natural fiber such as linen)

Limited amount of sample to adequately assess heterogeneity of the source

Minor explainable or demonstrable variation due to established causes such as damage (e.g., impact), alteration (e.g., heat or chemical exposure), or known contamination (e.g., biological fluids)

Circumstances where a narrow range of fiber type and color are likely to be encountered (e.g., same type of uniform worn by multiple people), which could lead to a random association

Reduced analytical scheme, damaged fibers, or limited sample size

Inconclusive

Some difference which may be due to questioned fiber being too damaged for full analysis, or

The questioned fiber possesses similar characteristics to the known sample but also exhibits some differences such as:

- Post-depositional changes
- Known sample not being truly representative



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 7 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Exclusion with Limitations

- Change or damage that could be from exposure to heat, chemicals or environmental effects
- Limited amount of known sample of a suspected source that is highly variable (e.g., trunk liner)
- Manufacturing variation/irregularities

Exclusion

- Different in microscopical, physical, and/or chemical properties

4.4. Paint

Type I Inclusion: Source Identification

The items exhibit physical features that demonstrate they were once part of the same object

Type II Inclusion: Inclusion with highly discriminating characteristics

Samples correspond in all chemical and physical characteristics and include characteristics atypical of most paint systems

- Multiple layer automotive paint with OEM and non-OEM layers
 - § OEM system with at least one aftermarket basecoat or primer layer above the original clear coat
 - § OEM system with 2 or more factory repairs (i.e., three or more total basecoat/clearcoat sequences)
 - § Automotive paint systems with architectural paint present
- Architectural paint with two or more different color layers

Type III Inclusion: Inclusion with discriminating characteristics

Samples correspond in all chemical and physical characteristics with typical analytical scheme

- Multiple layered OEM paints
- Non-automotive single-layered colored paint where there is knowledge of substantial discrimination power (e.g., red architectural paint) or product distribution information that reduces the potential sources
- Two or more white architectural layers of different chemistries

Type IV Inclusion: Inclusion with limitations

Samples correspond in all chemical and physical characteristics, but there is a limitation

- Lacking necessary analysis in typical analytical scheme
- Smears
- Single automotive paint (e.g., clear coat or unremarkable base coat such as a white color acrylic melamine binder system with primarily titanium dioxide as an extender pigment)
- Single-layer paint having limited discrimination studies or product manufacturing distribution information



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 8 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Inconclusive

Samples exhibit both similarities and differences such that no meaningful conclusion can be reached

- Sample with known contamination has a dissimilar elemental profile
- Questioned sample of spray paint can have differing pigment to binder ratios that cannot be reproduced from the small amount of paint left in the known spray can due to mixing differences
- Clear coat cross-transfer in which both known vehicles have indistinguishable clear coat chemistries

Exclusion with Limitations

Limited application to paint comparisons

- One sample of paint in a comparison has an extra layer (e.g., anti-chip layer). No analytical differences were observed in the corresponding layers. The vehicle is no longer available to collect an additional known sample

Exclusion

Compared paints are different in physical and/or chemical properties

4.5. Tape

Type I Inclusion: Source Identification

The items exhibit physical features that demonstrate they were once part of the same object

Type II Inclusion: Inclusion with highly discriminating characteristics

Unusual or distinctive features (e.g., not enough for a physical fit but has a defect or two) and corresponds in all other physical and chemical characteristics
Post-manufacturing marks such as damage, writing, or paint overspray

Type III Inclusion: Inclusion with discriminating characteristics

Samples correspond in all chemical and physical characteristics with typical analytical scheme

Type IV Inclusion: Inclusion with limitations

Limited analytical scheme due to sample size

Backing or adhesive only

Minor explainable or demonstrable variation in one of the comparison samples due to established causes such as:

- Sample heterogeneity of the scrim
- Known contamination of the sample(s)
- Having a sample of insufficient size to adequately assess the homogeneity of the entity from which it was derived

Inconclusive

No conclusion can be reached between the questioned and known samples

The questioned item is too damaged, degraded, or contaminated to conduct most examinations.



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 9 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Exclusion with Limitations

A conclusion not commonly used for tape exams

Exclusion

Compared tapes are different in physical and/or chemical properties

4.6. Other

Type I Inclusion: Source Identification

The items exhibit physical features that demonstrate they were once part of the same object

Type II Inclusion: Inclusion with highly discriminating characteristics

Samples correspond in all examined chemical and physical characteristics and have additional unusual features not expected for that type of material

- Example: Adhesive with similar extraneous material attached to it.

Two items physically fit together, but potentially lack enough detail or quality to state that no other item could also fit.

- Example: A match from a matchbook with no surrounding matches and indistinct tear that contains one single colored fiber traversing the tear.

Items that are too damaged to physically fit back together, but their breaks align.

Type III Inclusion: Inclusion with discriminating characteristics

Samples correspond in all examined chemical and physical characteristics
Match sticks or glitter

- Samples correspond in physical size, microscopic characteristics, and chemical composition (FTIR, elemental)

Coating

- A coating that has more than one layer

Type IV Inclusion: Inclusion with limitations

Samples correspond in all chemical and physical characteristics, but there is a limitation such as:

- Lack of features to compare
- Lack of discrimination studies or manufacturing knowledge
- Common material (e.g., hot melt glue, PVC pipe)

Only physical measurements taken (limited analytical scheme)

Single clear coating

Matchstick with only a portion remaining (e.g., head is not present for analysis)

Inconclusive

Samples exhibit similarities and differences such that no conclusion can be reached

Too little sample is available for comparison (known or questioned)

Exclusion with Limitations

Dissimilarities between known and questioned, but insufficient for a definitive exclusion due to limiting factors such as:



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 10 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

- Apparent contamination that cannot be removed or avoided in analysis
- Indications of change or damage that could be from exposure to heat

Exclusion

Different in physical, optical, and/or chemical properties

5. Activity level considerations

Activity level is an aspect of comparative examinations that considers factors such as transfer mechanisms and persistence. Factors include the presence of the evidence in a particular location, quantity and/or condition. Activity level can affect the significance of an association and may warrant additional statements within the report.

5.1. Activity level factors can include but are not limited to:

- Large number of items (e.g., fibers) transferred
- Location of evidence (e.g., underneath victim's fingernails)
- Multiple associations
- Cross transfer
- Conditions that limit the possible source (e.g., numerous fibers embedded in an interior surface of a vehicle with a known number of passengers)
- Reasonable explanation for a transfer of fibers (e.g., two individuals living together)
- Condition of evidence that indicates an activity (e.g., spray paint droplets indicate the paint applied wet to the surface as opposed to being smeared on an item after the paint was dry or stretched hair root may indicate it was forcibly removed)
- Evidence embedded rather than loosely adhered

5.2. Examples of activity level statements can be added to the report:

Number of pieces:

The large number of fibers recovered from Exhibit 1 indicates direct contact occurred with a textile.

The large number of glass fragments recovered from Exhibit 1 indicates a recent exposure to broken glass.

Physical characteristics:

The fibers embedded in the damaged area of the suspect vehicle indicate that the vehicle has been in forceful contact with a fabric-clad item.

Considering the presence of damaged fibers on the suspect fender consistent with the victim's jacket and pants, there is an indication of contact between the victim and the suspect vehicle.



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 11 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Although the fibers were blue denim cotton, which are commonly found in the environment, finding blue denim cotton fibers embedded in the damaged area of the vehicle lends more significance to their evidentiary value.

A clump of hairs, similar in color, found in the victim's hand all contained stretched roots and adhering tissue/root sheath which are indicative of the hairs having been forcibly removed.

The physical characteristics of the paint on Exhibit 1 establishes that the paint was sprayed on when applied.

Multiple or cross transfers:

Based on the results, four (4) distinct associations are reported. These findings provide stronger support for a common source than a single association alone and therefore, the overall significance of the reported results is increased due to the multiple associations.

Numerous fibers were found on the victim's shirt that could not be distinguished from the fibers comprising the known shirt from the subject. Numerous fibers were found on the subject's shirt that could not be distinguished from the fibers comprising the known shirt from the victim. This cross transfer provides stronger support for contact having occurred between the two shirts than either transfer alone and reduces the chance that the fibers were all deposited by coincidence.

6. Report wording examples

The following examples are meant to give guidance with regards to wording of trace evidence reports; however, exact wording should be left to the discretion of the examiner.

6.1. Type I Inclusion: Source Identification

Fiber (Fabric) wording examples:

*The torn edge of the questioned fabric piece physically fits and aligns with the torn edges of the known shirt fabric. This provides the strongest support that the fabric piece originated from and was at one time part of the shirt, as opposed to it originating from another torn fabric source (**Type I Inclusion**).*

*The Exhibit 1 and Exhibit 2 pieces of fabric corresponded in edge contour including yarn length characteristics that corresponded across the tear. This demonstrates that these two pieces of fabric were once part of a single unit (**Type I Inclusion**).*

Fabric impression wording example:



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 12 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

*The fabric impression from Exhibit 2 corresponded in construction, weave, and the presence of multiple holes to the known fabric from the Exhibit 1 jeans. Therefore, the Exhibit 1 jeans are the source of the fabric impression in Exhibit 2 (**Type I Inclusion**). This conclusion was reached because these distinct characteristics would not be expected to be repeated in another source.*

Paint wording example:

*Examination and comparison of Exhibits 1 and 2 revealed corresponding fracture contours, surface configurations, and layer structures of the two paint chips. This demonstrates that the items originated from the same damaged source (**Type I Inclusion**).*

Tape wording examples:

*Unknown duct tape fragments from the scene (Exhibits 1, 8 and 9) were visually and microscopically compared to the end of the roll of grey duct tape in Exhibit 4 and to each other. Multiple physical fits were made between the pieces of tape in Exhibits 1, 8 and 9 as well as a physical fit was made between one piece of duct tape in Exhibit 8 to the end of the roll of tape in Exhibit 4. Therefore, all of these pieces of tape including the roll of tape were at one time a single unit (**Type I Inclusion**).*

*Based on distinct features of the torn edge on one end of the Exhibit 1 piece of tape and the end of the roll in Exhibit 2, Exhibit 1 was observed to physically correspond with the end of Exhibit 2. This provides the strongest support that Exhibit 1 originated from and was at one time a part of Exhibit 2 as opposed to it originating from another used roll (**Type I Inclusion**).*

Other wording example:

*The Exhibit 1 and Exhibit 2 plastic fragments corresponded in edge contour and had surface scratches that corresponded across the break. This demonstrates that these two pieces of plastic were once part of a single unit (**Type I Inclusion**). This conclusion was reached because these alignments fit together in a manner that is not expected to be repeated in another source.*

6.2. Type II Inclusion: Inclusion with highly discriminating characteristics

Fiber wording example:

*The Exhibit 1 fibers were compared to the known fibers in Exhibit 2 and found to correspond in color and type (insert color and type here), microscopic characteristics, cross-section (insert shape), fluorescence, chemical composition. In addition, both Exhibits 1 and 2 corresponded in distinctive characteristics (list distinctive characteristics, e.g., damage indicative of singeing). Therefore, the Exhibit 1 fibers came from Exhibit 2 or another source having the same highly discriminating characteristics (**Type II Inclusion**). This type of association was reached because both Exhibit 1 and*



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 13 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Exhibit 2 display characteristics atypical of the relevant population of this evidence type. (Further description of the highly discriminating characteristics present are added here).

Fabric impression wording example:

*The impression from Exhibit 1 corresponded in construction and weave to the known shirt in Exhibit 2. In addition, there was an outline of a badge and some distinctive characteristics found in both the Exhibit 1 impression and the known shirt/badge in Exhibit 2. Therefore, the Exhibit 1 impression could have been made by the Exhibit 2 known shirt or another source having the same highly discriminating characteristics (**Type II Inclusion**).*

Paint wording example:

*Exhibit 1 was examined microscopically and contained a nine-layered paint chip that corresponded in color and layer structure (list layers), chemical composition, and elemental composition to the known paint in Exhibit 2. Therefore, the Exhibit 1 paint came from the same source as the Exhibit 2 known paint sample or another source having the same highly discriminating characteristics (**Type II Inclusion**). This type of association was reached because both Exhibit 1 and Exhibit 2 display characteristics atypical of original equipment manufacturer (OEM) paints [or atypical of the relevant population of this evidence type]. (Further description of the highly discriminating characteristics present are added here)*

Tape wording example:

*The tape in Exhibit 1 corresponded in construction, general appearance (color (list color), size, etc.) chemical composition, and elemental composition to the known tape roll in Exhibit 2. [Further description of the highly discriminating characteristics present shall be added.] Therefore, the Exhibit 1 tape could have come from the same source as the Exhibit 2 known tape roll or another source having the same highly discriminating characteristics (**Type II Inclusion**).*

Other wording examples:

*The match from Exhibit 1 corresponded in general physical characteristics and the break edges align [has highly discriminating characteristics] with the matchbook in Exhibit 2. This indicates that Exhibit 1 and Exhibit 2 were likely part of a single unit, however, due to [damage of the evidence, lacking detail, or other limitation] an identification is not possible (**Type II Inclusion**).*

6.3. Type III Inclusion: Inclusion with discriminating characteristics

Fiber wording example:

The Exhibit 1 fibers were compared to the known fibers in Exhibit 2 and found to correspond in color and type (insert color and type here), and microscopic



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 14 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

*characteristics. In addition, one fiber from within Exhibit 1 and Exhibit 2 were further analyzed and found to be similar in cross-section (insert shape) and chemical composition. Therefore, Exhibit 1 could have come from Exhibit 2 or another source with the same characteristics (**Type III Inclusion**). This type of conclusion was reached because other textiles containing fibers made to the same specifications (type, color, microscopic characteristics, etc.) would also be indistinguishable from these fibers. The techniques utilized in this comparative analysis can readily distinguish different fibers.*

Fabric damage wording example:

*The damage in the Exhibit 1 shirt was examined under the stereomicroscope and determined to be cut. Sample cuts, made by the Exhibit 2 pinking shears, were consistent in physical appearance (angles, lengths of angle segments, etc.) with the damage found in Exhibit 1. Therefore, the damage in Exhibit 1 could have been made by the Exhibit 2 pinking shears or another source with the same characteristics (**Type III Inclusion**). This conclusion was reached because other pinking shears with the same measurements could leave indistinguishable characteristics.*

Fabric impression wording example:

*The Exhibit 1 impression corresponded in construction and weave pattern as well as seam lines to the known pair of pants in Exhibit 2. Therefore, the known pants in Exhibit 2 could be the source of the impression in Exhibit 1 (**Type III Inclusion**). This type of conclusion was reached because other items (can list item type) may have been manufactured to the same specifications that would be indistinguishable from the submitted evidence.*

Paint wording example:

*The paint chip in Exhibit 1 was examined microscopically and corresponded in color and layer structure (list layers), chemical composition, and elemental composition to the known paint in Exhibit 2. Therefore, the Exhibit 1 paint could have come from the same source as Exhibit 2 or another source with the same characteristics (**Type III Inclusion**). This type of conclusion was reached because paints are mass-produced, and other paints manufactured to the same specifications as Exhibit 2 would also be indistinguishable from this paint. The techniques utilized in this comparative analysis can typically distinguish most paint products.*

Tape wording example:

*The piece of tape in Exhibit 1 corresponded in construction, general appearance (color (list color), size, etc.) chemical composition, and elemental composition to the known tape roll in Exhibit 2. Therefore, Exhibit 1 could have come from the same source as Exhibit 2 or another source with the same characteristics (**Type III Inclusion**). This type of conclusion was reached because other rolls of tape produced at the same manufacturing plant and with the same specifications would also be indistinguishable. Due to differences*



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 15 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

between tape products, the analytical techniques used in the analysis of these items allow for a high degree of discrimination.

Tape wording example:

*Ten pieces of white duct tape found at the scene (Exhibits 5, 6, 7 and 8) were compared to known white duct tape from Exhibit 32 (suspect's residence). No physical fits were made between any of the unknown white tape and the known roll of white tape. The unknown pieces of white duct tape in Exhibits 5, 6, 7 and 8 were similar to the known white duct tape in Exhibit 32 in construction and physical characteristics (color of backing, color of adhesive, scrim weave and width when available). In addition, one piece within Exhibit 6 and the known tape in Exhibit 32 were further analyzed. These tapes were also found to be similar in microscopic characteristics of adhesive and scrim fibers, scrim construction, chemical composition and elemental composition. Therefore, the unknown white duct tape analyzed from the scene (Exhibit 6) could have come from the known white duct tape in Exhibit 32 or another source having the same characteristics (**Type III Inclusion**). This type of conclusion was reached because other rolls of tape produced at the same manufacturing plant and with the same specifications would also be indistinguishable. Due to differences between tape products, the analytical techniques used in the analysis of these items allow for a high degree of discrimination.*

Other wording example:

*The matchsticks in Exhibits 1 and 2 from the scene were similar in color of shaft, size (length and width) and visual color of residue/match head material when visible. In addition, two matchsticks from Exhibit 1 and four matchsticks from Exhibit 2 were further analyzed and also found to be similar in microscopic characteristics of the wooden shaft, chemical composition, and elemental composition of the green residue/match head material. Therefore, the matchsticks in Exhibits 1 and 2 could have a common source however, other matchsticks may have been manufactured to the same specifications that would be indistinguishable from the submitted evidence (**Type III Inclusion**).*

6.4. Type IV Inclusion: Inclusion with limitations

Fiber wording example:

*The Exhibit 1 fibers were compared to the known fibers in Exhibit 2 and found to correspond in color and type (insert color and type) and chemical composition. Therefore, Exhibit 1 could have come from the same source as Exhibit 2 or another textile with the same characteristics (**Type IV Inclusion**). This conclusion is limited because this type of fiber [or list fiber type e.g., blue cotton] is ubiquitous and may have limited forensic value.*

Fiber wording example:

The Exhibit 1 fibers were compared to the known fibers in Exhibit 2 and found to correspond in (insert characteristics here). Therefore, Exhibit 1 could have come from the



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 16 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

*same source as Exhibit 2, however this association is limited due to [the sample size/the condition of the sample/being commonly encountered/a lack of characteristics available for comparison] (**Type IV Inclusion**). Other items may have fibers manufactured to the same specifications that would be indistinguishable from the submitted evidence.*

Fabric damage wording example:

*Exhibits 1 and 2 were examined with a stereomicroscope for fabric damage. Fabric damage was observed in Exhibits 1 and 2, which was determined to be consistent with being cut. In addition, the fabric damage exhibited characteristics that indicated the damage was caused by scissors. The Exhibit 3 scissors could be a possible source of this damage (**Type IV Inclusion**). This conclusion is limited because most straightedge scissors would be included as a possible source of the damage noted.*

Fabric impression wording example:

*The known shirt in Exhibit 2 corresponded in construction and weave pattern to the partial fabric impression in Exhibit 1. Therefore Exhibit 2 could be the source of the Exhibit 1 impression, however this association is limited due to the commonality of the fabric construction [or other limitation] in the Exhibit 1 impression (**Type IV Inclusion**). This type of conclusion was reached because other items (can list item type) may have been manufactured to the same specifications that would be indistinguishable from the submitted evidence.*

Paint wording example:

*The paint chip in Exhibit 1 was examined microscopically and corresponded (insert characteristics here) to the known paint in Exhibit 2. Therefore, Exhibit 1 could have come from the same source as Exhibit 2, however this association is limited due to [the sample size/the condition of the sample/being commonly encountered/a lack of characteristics available for comparison] (**Type IV Inclusion**). Other items [cars/tools/etc.] may have paint [paint systems] manufactured to the same specifications that would be indistinguishable from the submitted evidence.*

Tape wording example:

*The tape from Exhibit 2 corresponded in (insert characteristics here) to the known tape roll from Exhibit 1. Therefore, Exhibits 1 and 2 could have come from a common source; however, this association is limited due to [the sample size/ the condition of the sample/being commonly encountered/a lack of characteristics available for comparison] (**Type IV Inclusion**). (Optional) Other items [tape] may have been manufactured to the same specifications that would be indistinguishable from the submitted evidence.*

Other wording examples:

The matchstick in Exhibit 1 was compared to the matchsticks in Exhibits 2 and 3. The



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 17 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

*matchsticks were similar in shaft color, physical dimensions and microscopic characteristics. Therefore, the matchsticks in Exhibits 1, 2 and 3 cannot be eliminated as having a common source (**Type IV Inclusion**). This examination was limited due to the missing heads of the matches which can provide additional discrimination.*

*The Exhibit 1 lacquer recovered from the pipe was compared to the known lacquer sample from the suspect's garage (Exhibit 2). The samples were consistent in color (clear), chemical composition and elemental composition. Therefore, Exhibit 2 cannot be eliminated as a possible source of the questioned lacquer (**Type IV Inclusion**). This type of association was reached due to the limited characteristics available for comparison in clear lacquer. Other items may contain lacquer manufactured to the same specifications that would be indistinguishable from the submitted evidence.*

6.5. Inconclusive

Fiber wording example:

*The Exhibit 1 blue nylon fibers were compared to the blue nylon fibers from the Exhibit 2 known carpet and found to correspond in microscopic characteristics. However, slight differences were noted in the color between the Exhibits 1 and 2 fibers. Because of the questioned fibers' exposure to the elements, no conclusion can be reached regarding an association or exclusion between the questioned and known fibers (**Inconclusive**).*

Fabric damage wording example:

*The Exhibit 1 shirt contained damage that was determined to be consistent with a cut. In addition, there was additional damage of stretching. The Exhibit 2 knife was evaluated to determine if it could be the source of the damage on Exhibit 1. Due to the additional damage on the shirt, no conclusion can be reached regarding whether or not the Exhibit 2 knife could have made the cut in the Exhibit 1 shirt. (**Inconclusive**).*

Fabric impression wording example:

*The photographs on the Exhibit 1 CD contained images of a fabric impression, however the substrate that the impression was on interfered with the pattern. Therefore, no conclusion can be reached as to the source of the questioned impression (**Inconclusive**).*

Paint wording example:

*The paint in Exhibit 1 was examined microscopically and corresponded in color and layer structure (list layers) and chemical composition to the Exhibit 2 known sample. However, Exhibits 1 and 2 differed slightly in elemental composition which could be due to the heterogeneity of paint or because the samples are from different sources. Therefore, no conclusion can be reached regarding the inclusion or elimination of these paint samples (**Inconclusive**). [Include any relevant limitations to this examination that may have contributed to the inconclusive conclusion]*



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 18 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Tape wording example:

*The tape from Exhibit 1 corresponded in general appearance and chemical composition to the known tape in Exhibit 2; however, the elemental composition of the adhesive was slightly different from the known due to possible contamination. Therefore, no conclusion can be reached regarding the association of these tape samples (**Inconclusive**). [Include any relevant limitations to this examination that may have contributed to the inconclusive conclusion]*

6.6. Exclusion with Limitations

Fiber wording example:

*Questioned fibers were compared to fibers composing the samples from the known trunk liner using (insert methods here). The questioned fibers were different in (insert characteristics here) to the fiber samples from the known trunk liner, indicating the items did not originate from the same source; however, possible reasons for this difference include that the source is highly variable, and the fiber samples provided may not be representative. Therefore, this difference is insufficient for an exclusion conclusion (**Exclusion with Limitations**).*

Fabric damage wording example:

*The holes in Exhibit 1 were examined with a stereomicroscope and determined to be consistent with a cut. The holes were all less than 1 centimeter in length. The knives in Exhibits 2 and 3 were compared to the damage in Exhibit 1. The single edge blade in Exhibit 2 could be a source of the holes in Exhibit 1 (**Type III Inclusion**). The single edge blade in Exhibit 3 was wider and all of the sample cuts produced larger holes. However, due to the possibility only the tip of Exhibit 3 made the cuts, an exclusion conclusion could not be made (**Exclusion with Limitations**).*

Fabric impressions wording example:

*Exhibit 1 has a similar pattern to the questioned impression from Exhibit 2, but there were minor differences [list differences] in the pattern and therefore, Exhibit 1 may not be the source (**Exclusion with Limitations**).*

Fabric impressions wording example:

*The pattern seen in the questioned impression shows some similarity to the known item, however, test impressions made with the known could not replicate the exact pattern. Therefore, it is unlikely that the known pants made the questioned impression (**Exclusion with Limitations**).*

6.7. Exclusion



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 19 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

Fiber wording example:

*Fibers from Exhibit 1 were compared to the known fibers in Exhibit 2. These fibers were different in microscopic characteristics [insert characteristics that differ]. Therefore, the Exhibit 1 fibers did not come from Exhibit 2 (**Exclusion**).*

Fiber wording example:

*The fibers from Exhibits 1 and 2 were compared and although visibly similar in color (list color), their fiber types were different. Exhibit 1 was determined to be polyester, and Exhibit 2 was determined to be polypropylene. Therefore, the Exhibit 1 fibers did not come from Exhibit 2 (**Exclusion**).*

Fabric damage wording example:

*The damage in the Exhibit 1 shirt was examined under a stereomicroscope and determined to be cut. Sample cuts made by the Exhibit 2 scissors produce damage different from that found in Exhibit 2. Therefore, the damage in Exhibit 1 was not made by Exhibit 2 (**Exclusion**).*

Fabric impression wording example:

*The pattern seen in the Exhibit 1 questioned impression was different from the known fabric from Exhibit 2 and therefore, can be excluded as being a possible source for the Exhibit 1 impression (**Exclusion**).*

Paint wording example:

*The paint chip in Exhibit 1 displayed a different color and layer structure than the known paint in Exhibit 2. Therefore, the Exhibit 1 paint did not come from the known sample in Exhibit 2 (**Exclusion**).*

Paint wording example:

*The paint chips in Exhibit 1, though visibly similar in color and layer structure, are different in chemical composition from the known paint in Exhibit 2. Therefore, the paint in Exhibit 1 did not come from the same source as the Exhibit 2 known paint (**Exclusion**). Different panels on the same vehicle may have different paint systems. Further comparisons can be performed if additional known samples are submitted.*

Tape wording example:

*The tape in Exhibit 1 displayed a different color and chemical composition than the known tape roll in Exhibit 2. Therefore, the Exhibit 1 tape did not come from the known tape in Exhibit 2 (**Exclusion**).*

Other wording example:

*The piece of plastic from Exhibit 1 was a different color than the Exhibit 2 bumper. Therefore, Exhibit 2 can be eliminated as the source of Exhibit 1 (**Exclusion**).*



ATF-LS-TE16 Report Writing	ID: 1935 Revision: 7
Authority: Technical Leader	Page: 20 of 20
Original maintained by Quality Programs; copies are uncontrolled.	

7. References

- 7.1 ASTM International. *ASTM E620 Standard Practice for Reporting Opinions of Technical Experts*. ASTM International, West Conshohocken, Pennsylvania. Available: <http://www.astm.org/Standards/E620.htm>.
- 7.2 ASTM International. *ASTM E678 Standard Practice for Evaluation of Scientific or Technical Data*. ASTM International, West Conshohocken, Pennsylvania. Available: <http://www.astm.org/Standards/E678.htm>.
- 7.3 International Organization for Standardization/International Electrotechnical Commission (ISO/IEC). *ISO/IEC 17025:2017 General Requirements for the Competence of Testing and Calibration Laboratories*. ISO/IEC, Geneva, Switzerland.
- 7.4 ANAB ISO/IEC 17025:2017 – Forensic Science Testing and Calibration Laboratories Accreditation Requirements AR 3125.
- 7.5 Organization of Scientific Area Committees for Forensic Science (OSAC) Materials Subcommittee Draft Standard Practice for Interpretation and Report Writing in Forensic Comparison of Trace Materials, May 2020 [Online]. Available at: <https://www.nist.gov/system/files/documents/2020/04/02/ChSAC-Mat Interpretation Document March2020 0.pdf>
- 7.6 Department of Justice policy on Uniform Language for Testimony and Reports available at www.justice.gov



ATF-LS-TE17 Trace Abbreviations	ID: 10199 Revision: 2
Authority: Technical Leader	Page: 1 of 3
Original maintained by Quality Programs; copies are uncontrolled.	

Abbreviations

approx
ATR
B
BPB
BPT
BT
C
cont
EDS
Env, ENV
Ex, Exh
ER
ET
Frag(s)
FTIR
GET
GT
HS
I&D
in
IR
IU
K
lg
ME
med
min
mDNA, mtDNA
MS
MSP, Microspec
μscope
n/a
n_{||}
n_⊥
nDNA, nucDNA
neg, (-)
nm
NSR
PB
PC
PLM

Description

Approximately
Attenuated total reflectance
Birefringence
brown paper bag
brown paper tape
brown tape
contrast
contained, contains, container
energy dispersive x-ray spectroscopy
envelope
Exhibit
Exam Request, Evidence Room
evidence tape
fragment(s)
Fourier Transform Infrared Spectroscopy
green evidence tape
green tape
heat sealed
initialed and dated
inches
infrared
initials unidentified
known
large
manila envelope
medium
minutes
Mitochondrial DNA
mass spectrometer
Microspectrophotometer
Microscope
non-applicable
refractive index - parallel
refractive index - perpendicular
Nuclear DNA
negative
nanometer
no significant reaction
plastic bag, post blast
paint chip
polarized light microscopy



ATF-LS-TE17 Trace Abbreviations	ID: 10199 Revision: 2
Authority: Technical Leader	Page: 2 of 3
Original maintained by Quality Programs; copies are uncontrolled.	

Abbreviations

pos, (+)
poss
prep
PGC, PyGC
Q
QC
R
RET
rep(s)
RB
RI
RL
S
SD
SEM
sm
SOE
std
temp
T
TL
unk
UV
w/
w/o
WET
X
XRD
XRF
YET
ZLB
(“abc”)

Description

positive
possible
prepare
pyrolysis gas chromatography
questioned
quality check, quality control
retardation, radial section
red evidence tape
repetition
red-brown
refractive index
reflected light
sealed
standard deviation
scanning electron microscope
small
sign of elongation
standard
temperature
tangential section
transmitted light
unknown
ultra-violet
with
without
white evidence tape
cross section
X-ray diffraction
X-ray fluorescence spectroscopy
yellow evidence tape
zip lock bag
initialed with legible letters

Additional symbols on following page



ATF-LS-TE17 Trace Abbreviations	ID: 10199 Revision: 2
Authority: Technical Leader	Page: 3 of 3
Original maintained by Quality Programs; copies are uncontrolled.	

Symbol

λ

\sim

$=$

\approx, \cong

\perp

\parallel

\gg

$>$

\geq

\leq

$<$

\ll

\therefore

Description

wavelength

about, approximately

equal to, consistent with

similar to, approximately equal to, consistent with

perpendicular

parallel

Much greater than

Greater than

Greater than, but nearly equal

Less than, but nearly equal

Less than

Much less than

therefore